

15TH TOPICAL SEMINAR ON INNOVATIVE PARTICLE AND RADIATION DETECTORS
 WHEN 14-17 OCTOBER 2019
 WHERE SIENA, ITALY

Studies on tetrafluoropropene-based gas mixtures with low environmental impact for Resistive Plate Chambers

A. Bianchi,^{a,1} S. Delsanto,^a P. Dupieux,^b A. Ferretti,^a M. Gagliardi,^a B. Joly,^b S. P. Manen,^b M. Marchisone,^c L. Micheletti,^a A. Rosano^a and E. Vercellin^a

^a*Università degli Studi di Torino and INFN, Sezione di Torino, Via Pietro Giuria 1, 10125, Torino, Italy*

^b*Clermont Université, Université Blaise Pascal, CNRS/IN2P3, Laboratoire de Physique Corpusculaire, BP 10448, F-63000 Clermont-Ferrand, France*

^c*Institut de Physique Nucléaire de Lyon, Université Claude Bernard, 4 rue Enrico Fermi, 69622, Villeurbanne, France*

E-mail: antonio.bianchi@unito.it

ABSTRACT: Gaseous detectors are widely used in high-energy physics experiments, and in particular at the CERN Large Hadron Collider (LHC), to provide tracking and triggering over large volumes. It has been recently estimated that Resistive Plate Chambers (RPC), used for muon detection, have the highest contribution on the overall greenhouse gas (GHG) emissions at the LHC experiments.

Gas mixtures for RPCs are mainly made of $C_2H_2F_4$, which is a greenhouse gas with a high environmental impact in the atmosphere. $C_2H_2F_4$ is already phasing out of production, due to recent European Union (EU) regulations, and its cost is expected to increase in the near future. Therefore, finding alternative gas mixtures made of gas components with a low Global Warming Potential (GWP) has become extremely important for limiting the GHG emissions as well as for economic reasons.

The novel hydrofluoroolefins are likely appropriate candidates to replace $C_2H_2F_4$ due to their similar chemical structures. This study is focused on the characterization of innovative gas mixtures with tetrafluoropropene HFO1234ze(E) ($C_3H_2F_4$) that is one of the most eco-friendly hydrofluoroolefins, thanks to its very low GWP. HFO1234ze(E)-based gas mixtures with the addition of Ar, N_2 , O_2 and CO_2 are extensively discussed in this paper as well as the role of $i-C_4H_{10}$ and SF_6 in such mixtures.

KEYWORDS: Resistive-plate Chambers, Gaseous Detectors, Eco-friendly Gas Mixtures

¹Corresponding author.

Contents

1	Introduction	1
2	RPC operation with environment-friendly gases	2
2.1	Experimental set-up	2
2.2	Methodology	3
3	Characterization of C₃H₂F₄-based gas mixtures with addition of Ar, N₂ or O₂	4
4	Characterization of C₃H₂F₄-based gas mixtures with CO₂	5
4.1	C ₃ H ₂ F ₄ -based gas mixtures with addition of CO ₂ and <i>i</i> -C ₄ H ₁₀	7
4.2	C ₃ H ₂ F ₄ -based gas mixtures with addition of CO ₂ and SF ₆	7
5	Conclusions	8

1 Introduction

Gaseous detectors are widely used in high-energy physics experiments, and in particular at the CERN Large Hadron Collider (LHC), to provide tracking and triggering over large volumes. It has been recently estimated that Resistive Plate Chambers (RPC), used for muon detection, have the highest contribution on the overall greenhouse gas (GHG) emissions at the LHC experiments [1]. RPC detectors are operated with a large fraction (between 89% and 95%) of tetrafluoroethane C₂H₂F₄, whose trade name is R-134a. In addition, different concentrations of *i*-C₄H₁₀ and SF₆ are used in RPC gas mixtures with the aim to optimize the detector performance. In the case of RPCs at the ATLAS and CMS experiments, the concentrations of *i*-C₄H₁₀ and SF₆ are 4.5% and 0.3%, respectively, while the ALICE gas mixture contains 10.0% *i*-C₄H₁₀ and 0.3% SF₆.

A greenhouse gas is classified according to its Global Warming Potential (GWP). This potential indicates the heat trapped by a gas in the atmosphere thus contributing to the greenhouse effect. The GWP of CO₂ is equal to 1 by definition. On the contrary, the GWPs of C₂H₂F₄ and SF₆ are 1430 and 22800, respectively, whereas the GWP of *i*-C₄H₁₀ is 3 [2]. This implies that the GWP of the ATLAS/CMS gas mixture is ~1430, while the GWP of the gas mixture used for the ALICE muon RPCs is ~1351.

Recent regulations from the European Union (EU) impose a gradual limitation of the production and usage of fluorinated greenhouse gases (such as C₂H₂F₄) [2]. This could lead to a progressive price increase of these gases. Therefore, finding gas mixtures made of low GWP components has become extremely important for limiting the GHG emissions in the atmosphere as well as for economic reasons. The new gas mixtures for RPCs must at least provide similar detector performance as the current ones.

In this paper we report the results of R&D studies on eco-friendly gas mixtures for RPCs, used for the muon detection, at the LHC experiments.

The paper is organized as follows. In section 2 we discuss the approach to find alternative, environment-friendly, gas mixtures. The characterization of $C_3H_2F_4$ -based gas mixtures with addition of the most common atmospheric gases is presented in section 3, whereas the measurements of detector performance with gas mixtures of $C_3H_2F_4$ and CO_2 are reported in section 4. Finally, conclusions are drawn in section 5.

2 RPC operation with environment-friendly gases

RPC gas mixtures, currently used at the LHC experiments, are not environment-friendly because of the presence of greenhouse gases. More than 95% of the total GWP of RPC gas mixtures at LHC is due to the presence of $C_2H_2F_4$.

The replacement of $C_2H_2F_4$ with tetrafluoropropene $C_3H_2F_4$ turns out to be a promising approach to find a more eco-friendly gas mixture [3–6]. Isomers of tetrafluoropropene are HFO1234ze(Z), HFO1234ze(E) and HFO1234yf. The most interesting isomer for the purposes of these R&D studies is the trans-1,3,3,3-tetrafluoroprop-1-ene HFO1234ze(E) because it has a low boiling point ($-19\text{ }^{\circ}\text{C}$) and is not flammable below $30\text{ }^{\circ}\text{C}$. The GWP of HFO1234ze(E) is 7 according to EU regulations [2], which is ~ 200 times lower than that of $C_2H_2F_4$. More recent studies have revised the GWP of HFO1234ze(E) to less than 1 [7]. In addition, it has been estimated that the decay products of HFO1234ze(E) in the atmosphere have a negligible environmental impact [8].

R&D studies on RPCs have been performed with HFO1234ze(E)-based gas mixtures. Hereafter, HFO1234ze(E) will be simply named as $C_3H_2F_4$ in order to be consistent with the chemical notation recognized by IUPAC¹ and used for all other gases in this work. Detector performance of single-gap RPCs of the ALICE muon spectrometer [9, 10] will be used as reference in this work.

2.1 Experimental set-up

A detailed description of the experimental set-up is presented in a previous work [11], while in this paper we only introduce its fundamental aspects.

R&D studies on various gas mixtures are carried out through one small-size ($50 \times 50\text{ cm}^2$, 2 mm gas gap) RPC with similar features as the ALICE muon RPCs [9, 10]. The ALICE muon RPCs have electrodes in phenolic bakelite with a resistivity of $10^9 \div 10^{10}\text{ }\Omega\text{ cm}$ [12], separated by a gas gap of 2 mm. The standard ALICE mixture is 89.7% $C_2H_2F_4$, 10.0% $i\text{-C}_4\text{H}_{10}$ and 0.3% SF_6 [13]. The relative humidity of the gas mixture is kept constant at $\sim 37\%$ with the aim to prevent variations of the electrode resistivity [14, 15].

In the experimental set-up, the detector is exposed to the cosmic-ray flux and equipped with the amplified front-end electronics FEERIC [16]. FEERIC amplifies signals up to $\pm 1\text{ pC}$ in the linear range [16], which is the typical input charge expected for the RPCs in avalanche mode. The four adjacent strips covering the trigger area are read out on both ends: on one end the signals are discriminated by FEERIC with the aim to assess the efficiency, while on the other end the analogic

¹International Union of Pure and Applied Chemistry

signals are summed by a fan-in/fan-out module and then digitized by an oscilloscope (LeCroy WaveSurfer 510) in order to measure the signal amplitude [11].

Figure 1 shows a sketch of the experimental set-up.

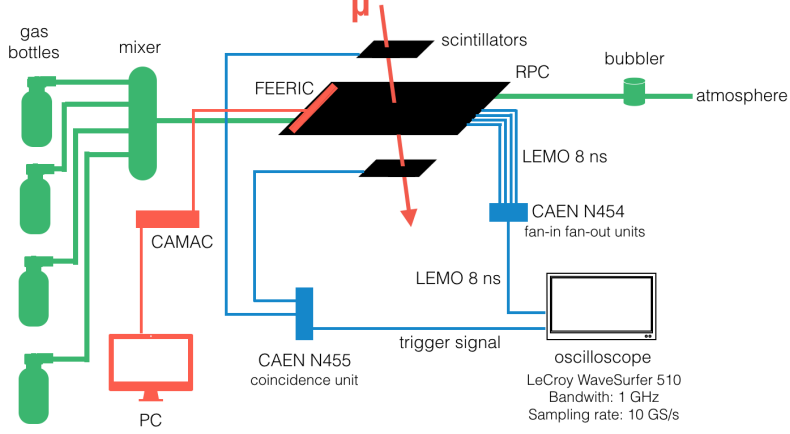


Figure 1. Sketch of the experimental set-up to measure the detector performance with $C_3H_2F_4$ -based gas mixtures.

2.2 Methodology

The new gas mixture with low GWP has to provide similar detector performance as the current one with the standard ALICE mixture. In this work, the working point, the fraction of streamers, the average charge of signals and the current stability are used to assess the performance of the tested gas mixtures.

The efficiency of the RPC detector is evaluated by analyzing the FEERIC response in each strip in the presence of a trigger signal [11]. The FEERIC discrimination threshold is ~ 130 fC (70 mV after the FEERIC amplification [17]). This threshold has been selected equal to the value used in one RPC of the ALICE muon identification system, equipped with FEERIC prototypes, with fully satisfactory performance during the data taking a period from 2015 to 2018 [17].

Signals with an amplitude higher than 18 mV are tagged as streamers [11]. Streamers are not desirable when RPCs are operated in avalanche mode because they reduce the rate capability of the detector [18] and may enhance ageing effects [15].

In figure 2 the efficiency curve² and the streamer probability versus HV is shown for the ALICE mixture and for pure $C_3H_2F_4$.

For the tested RPC, the efficiency plateau is reached at ~ 9.8 kV when the detector is equipped with FEERIC and flushed with the ALICE mixture. The streamer probability is about 5% at ~ 9.8 kV. On the contrary, the direct replacement of the ALICE mixture with 100% $C_3H_2F_4$ is not advisable

²The efficiency curves as a function of HV are fitted by the following sigmoid function:

$$\epsilon(HV) = \frac{\epsilon_{\max}}{1 + \exp[-\alpha \cdot (HV - HV_{0.5})]} \quad (2.1)$$

where ϵ_{\max} is the efficiency for $HV \rightarrow \infty$, $HV_{0.5}$ is the HV value for which the efficiency is equal to a half of ϵ_{\max} and α is the slope at the inflection point [11].

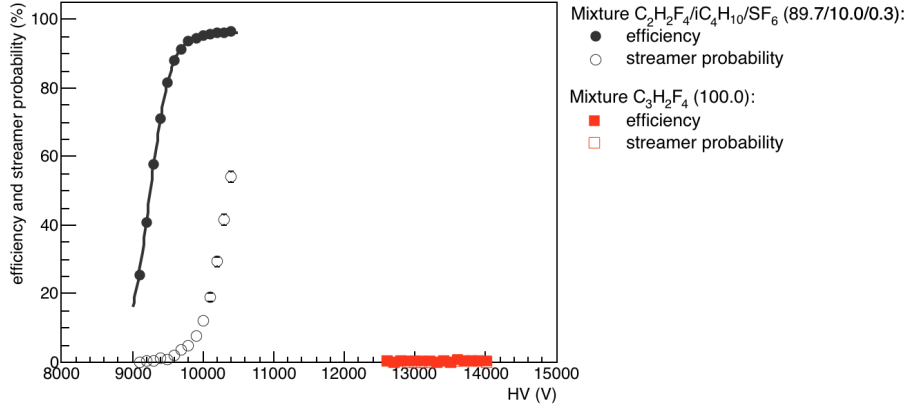


Figure 2. Efficiency curve and streamer probability of a RPC detector with the standard ALICE mixture and with pure $C_3H_2F_4$. Statistical error bars are hidden by markers.

because it leads to a too high operating voltage. Indeed, the RPC with 100% $C_3H_2F_4$ is completely inefficient up to 14 kV, as shown in figure 2.

In this work, $C_3H_2F_4$ is diluted with Ar, N_2 , O_2 and CO_2 in order to reduce the operating voltage of the detector.

3 Characterization of $C_3H_2F_4$ -based gas mixtures with addition of Ar, N_2 or O_2

The most common atmospheric gases have been tested in $C_3H_2F_4$ -based gas mixtures in order to lower the working point of RPCs. In particular, the study is here focused on Ar, N_2 and O_2 as their GWP is 0.

Figure 3 shows the experimental results of the efficiency and streamer probability curves of the RPC with 45% $C_3H_2F_4$ and the remaining fraction of Ar, N_2 or O_2 . As shown in figure 3a, the RPC operating voltages with $C_3H_2F_4$ -based gas mixtures and addition of Ar, N_2 and O_2 turn out to be extremely lower than that measured with pure $C_3H_2F_4$. In particular, the efficiency curve with Ar is at lower HV values by ~ 200 V in comparison to that with the standard ALICE mixture. On the contrary, the RPC working point with 55% O_2 and 45% $C_3H_2F_4$ is ~ 1.0 kV higher than that with the standard ALICE mixture, while the use of N_2 in place of O_2 shifts the working point by 1.5 kV. In figure 3b, the streamer probability curves are shown as a function of $HV - HV_{\epsilon=0.9}$. $HV_{\epsilon=0.9}$ is the voltage where the efficiency is 90% of its maximum value (ϵ_{max}), and is obtained, for each mixture, by fitting the efficiency curve with a sigmoid function. No significant changes in the streamer suppression are observed if 55% Ar, N_2 or O_2 is added to $C_3H_2F_4$. In fact, the streamer probability is always greater than $\sim 80\%$ at $HV - HV_{\epsilon=0.9}$ of ~ 200 V, while it is only $\sim 5\%$ in the standard ALICE mixture.

The average charge of RPC signals, induced in the read-out strips, has been measured at the working point in $C_3H_2F_4$ -based gas mixtures with 55% Ar, N_2 or O_2 . In order to measure this quantity for each gas mixture under test, RPC signals are acquired by the oscilloscope and then integrated in a time window of 100 ns by including each signal totally. At the working point, the average charge is ~ 2.6 pC with the standard ALICE mixture, while it turns out to be more than one order of magnitude higher in all other gas mixtures. In particular, the average charge is ~ 66 pC and

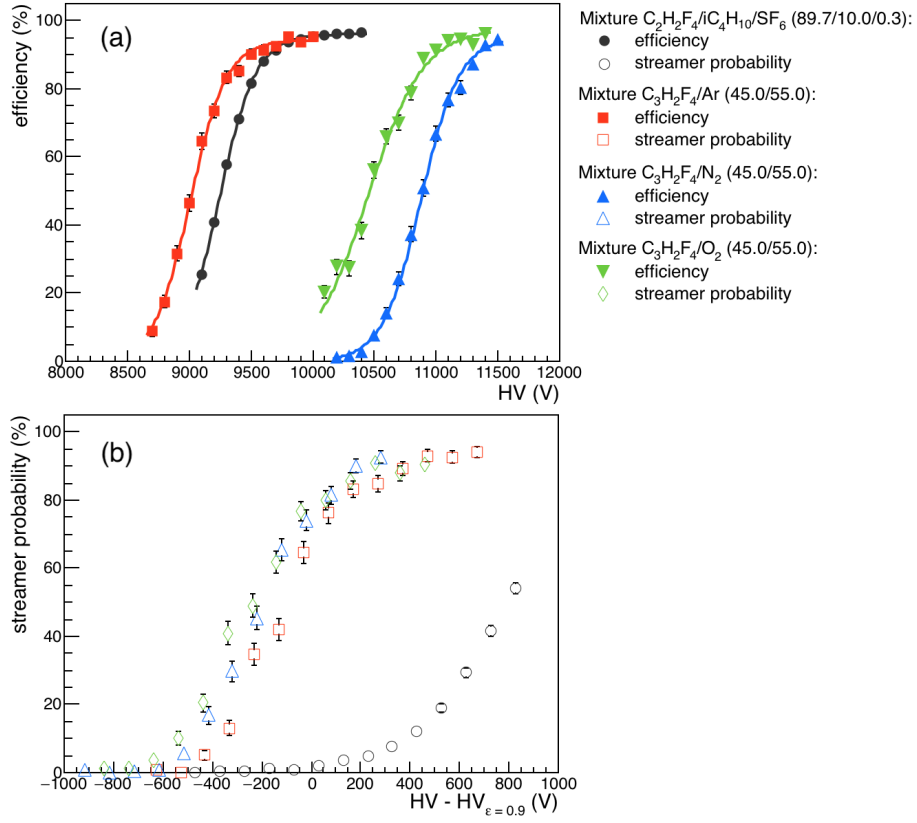


Figure 3. Efficiency (a) and streamer probability (b) of the RPC with 45% $C_3H_2F_4$ and the remaining fraction of Ar, N_2 or O_2 . In addition, the efficiency and the streamer probability of the RPC with the standard ALICE mixture are shown. Some statistical error bars are hidden by markers.

~68 pC in $C_3H_2F_4$ -based gas mixtures with 55% Ar and 55% N_2 , respectively. On the contrary, a lower average charge of ~36 pC is measured with 55% O_2 . However, a current instability has been observed if the RPC operates with 45% $C_3H_2F_4$ and 55% O_2 . In fact, the current at the working point increases by ~60% in 5 hours. The instability of the detector current has been observed in all $C_3H_2F_4$ -based gas mixtures with O_2 in different concentrations, tested so far.

4 Characterization of $C_3H_2F_4$ -based gas mixtures with CO_2

Since Ar, N_2 and O_2 do not turn out to be suitable in $C_3H_2F_4$ -based gas mixtures for RPCs, the use of CO_2 is here evaluated.

Figure 4a shows the efficiency curves of RPC at different ratios between $C_3H_2F_4$ and CO_2 .

If the gas mixture with 45% $C_3H_2F_4$ and 55% CO_2 is taken into consideration, the working point of the detectors is ~1.0 kV higher than that with the standard ALICE mixture. A similar effect has been already obtained in the gas mixture of 45% $C_3H_2F_4$ and 55% O_2 , as shown in figure 3. The streamer probability in the gas mixture with 55% CO_2 is ~50% at 90% efficiency, as shown in figure 4b. This value is lower than the streamer probability obtained in $C_3H_2F_4$ -based gas mixtures with the addition of 55% Ar, N_2 or O_2 , while it is still far from the value in the standard ALICE

mixture. Indeed, the streamer probability with 45% $\text{C}_3\text{H}_2\text{F}_4$ and the remaining fraction of Ar, N_2 or O_2 is $\sim 80\%$ at 90% efficiency, while it is less than 5% in the standard ALICE mixture. In the mixture with 55% CO_2 , the average signal charge is ~ 27 pC at the working point (11.2 kV), which is one order of magnitude greater than that of the standard ALICE mixture.

If the fraction of CO_2 is increased and that of $\text{C}_3\text{H}_2\text{F}_4$ is decreased, the working point turns out to be shifted towards lower voltages. Increasing the CO_2 fraction from 45% to 55% reduces the working point by ~ 1 kV. Figure 4b shows the streamer probability as a function of $HV - HV_{\epsilon=0.9}$. The increase of $\text{C}_3\text{H}_2\text{F}_4$ fraction against CO_2 reduces streamers. In fact, going from 45% to 55% $\text{C}_3\text{H}_2\text{F}_4$, the streamer probability at 90% efficiency decreases from $\sim 40\%$ to $\sim 20\%$.

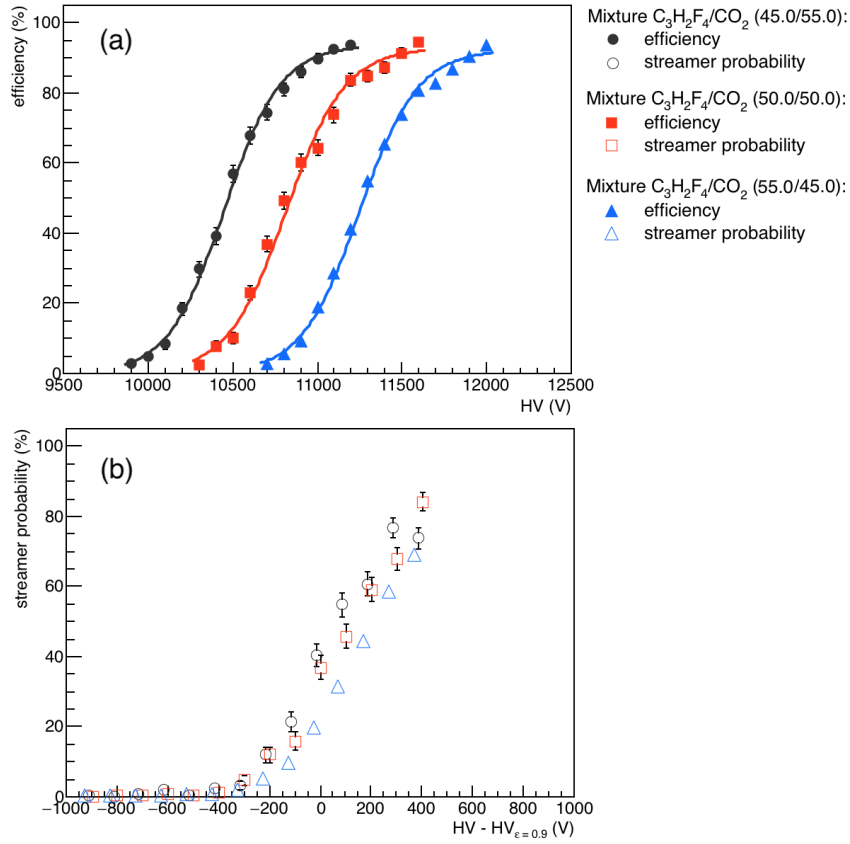


Figure 4. Efficiency (a) and streamer probability (b) of the RPC with $\text{C}_3\text{H}_2\text{F}_4$ -based gas mixtures and 45%, 50% or 55% CO_2 . Some statistical error bars are hidden by markers.

Taking into account the RPC working point, the streamer probability and the average charge of signals, CO_2 turns out to be the most promising solution in comparison to Ar, N_2 and O_2 . However, the streamer probability is quite high in gas mixtures with only $\text{C}_3\text{H}_2\text{F}_4$ and CO_2 , so results with the addition of $i\text{-C}_4\text{H}_{10}$, which has a high photo-absorption cross section, and addition of SF_6 , which is a strong electronegative gas, are presented in the following.

4.1 $C_3H_2F_4$ -based gas mixtures with addition of CO_2 and $i-C_4H_{10}$

The use of $i-C_4H_{10}$ in the $C_3H_2F_4$ -based gas mixtures for RPCs helps to reduce the photon-feedback effects, thanks to its high photo-absorption cross section [18].

Figures 5a and 5b show the efficiency and streamer probability curves, respectively, at different ratios between $i-C_4H_{10}$ and CO_2 , while the concentration of $C_3H_2F_4$ is kept constant at 45%. The working point increases by ~ 600 V when going from 10% to 20% $i-C_4H_{10}$, while no clear trend emerges when the $i-C_4H_{10}$ fraction is varied between 0% and 10%. The streamer suppression is more efficient with $i-C_4H_{10}$ concentrations higher than 10%. Indeed, streamer probability at 90% efficiency is $\sim 40\%$ without $i-C_4H_{10}$ or with 5% $i-C_4H_{10}$, while it is lower than 20% with more than 10% $i-C_4H_{10}$.

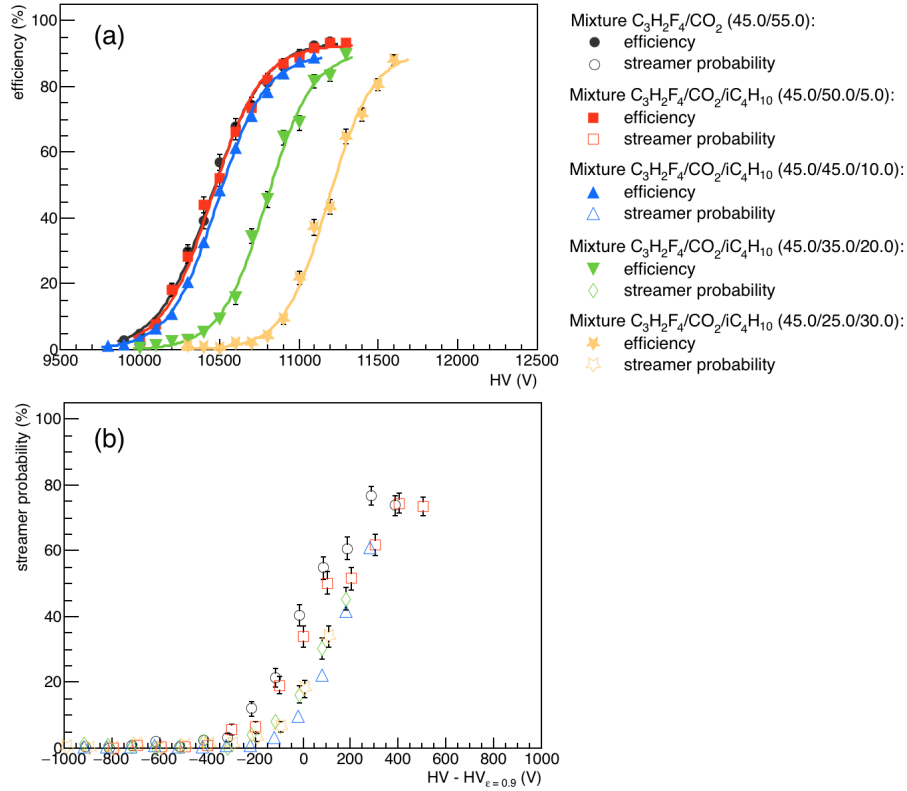


Figure 5. Efficiency (a) and streamer probability (b) of the RPC with 45% $C_3H_2F_4$ and different ratios between CO_2 and $i-C_4H_{10}$. Some statistical error bars are hidden by markers.

4.2 $C_3H_2F_4$ -based gas mixtures with addition of CO_2 and SF_6

The effect of 1% SF_6 has been tested in a gas mixture with only $C_3H_2F_4$ and CO_2 . Thanks to its high attachment cross sections [19], the addition of SF_6 in $C_3H_2F_4$ -based gas mixtures allows the suppression of streamers [20].

Figure 6 shows how the efficiency curve and the streamer probability change if 1% SF_6 is added to a gas mixture made of half $C_3H_2F_4$ and half CO_2 . The shift of the working point is ~ 1 kV towards higher voltages with the addition of 1% SF_6 . As expected, the streamers are greatly suppressed

with SF₆. Indeed, the streamer probability at 90% efficiency is ~40% without SF₆, whereas it is reduced down to ~5% with 1% SF₆.

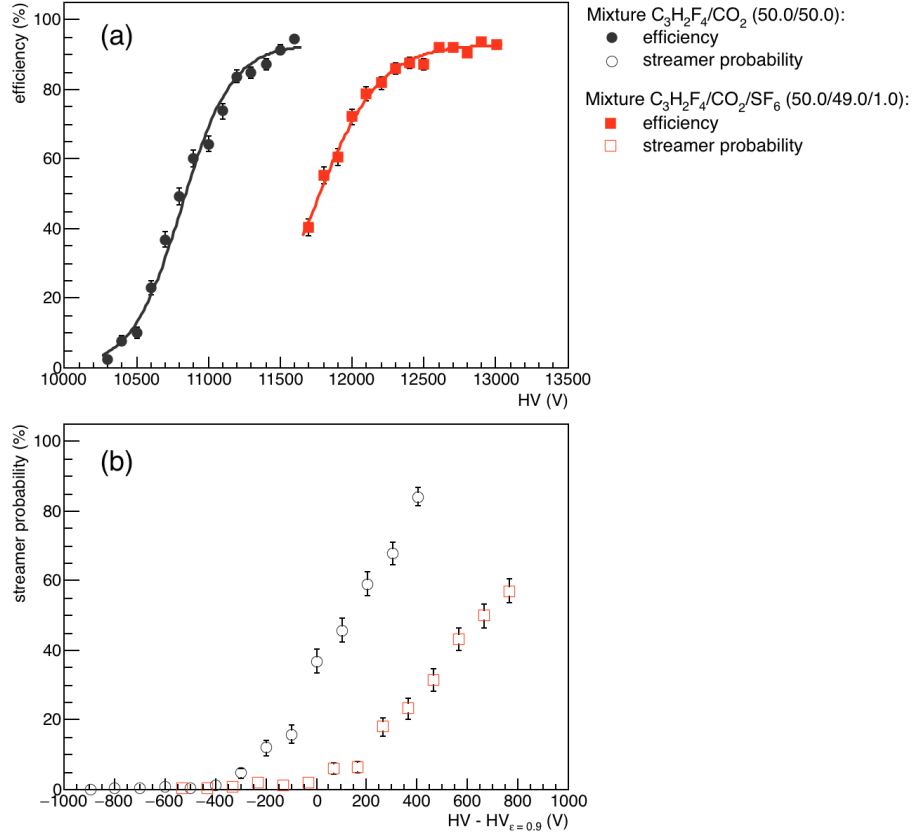


Figure 6. Efficiency (a) and streamer probability (b) of the RPC in C₃H₂F₄-based gas mixtures and CO₂ with and without the addition of 1% SF₆. Some statistical error bars are hidden by markers.

The addition of 1% SF₆ reduces also the average charge of signals. At the working point, the average charge is ~33 pC in the gas mixture of 50% C₃H₂F₄ and 50% CO₂, while it becomes only ~4 pC in the gas mixture with 1% SF₆.

5 Conclusions

The basic performance of C₃H₂F₄-based gas mixtures for RPCs have been studied. The usage of 100% C₃H₂F₄ in RPCs is not advisable because it leads to a too high operating voltage, as discussed in section 2.2.

The addition of Ar, N₂, O₂ and CO₂ in C₃H₂F₄-based gas mixtures reduces the operating voltage of the detector. However, the use of Ar, N₂ and O₂ in C₃H₂F₄-based gas mixtures implies high streamer probability and signal charge at the operating voltage. In addition, current instability is observed with the use of O₂ in the gas mixture.

CO₂ turns out to be the most promising solution. Indeed, values of streamer probability and signal charge are lower than those obtained in C₃H₂F₄-based gas mixtures with addition of Ar, N₂ and O₂, as shown in section 3. No current instability has been observed in any of the C₃H₂F₄-based

gas mixtures with CO₂, tested so far. Measurements with gas mixtures made of C₃H₂F₄ and CO₂ show that the addition of both *i*-C₄H₁₀, as quencher, and SF₆, as strong electronegative gas, improves the RPC performance.

The interplay of C₃H₂F₄, CO₂, *i*-C₄H₁₀ and SF₆ has been already investigated for single-gap RPCs in avalanche mode [11]. The most promising gas mixtures, which have been found so far [11], consist of 50% CO₂, 39.7% C₃H₂F₄, 10% *i*-C₄H₁₀, 0.3% SF₆ and 50% CO₂, 39% C₃H₂F₄, 10% *i*-C₄H₁₀, 1% SF₆. Their GWPs are respectively 72 and 232, while the GWP of gas mixtures for RPCs in muon detection systems of the LHC experiments is ~1400.

Measurements of the RPC performance under irradiation are ongoing at the CERN Gamma Irradiation Facility [21] in order to assess the rate capability and ageing properties resulting from the C₃H₂F₄-based gas mixtures.

References

- [1] M. Capeans, R. Guida, and B. Mandelli, *Strategies for reducing the environmental impact of gaseous detector operation at the CERN LHC experiments*, Nuclear Instruments and Methods in Physics Research Section A, 845:253–256, 2017
- [2] The European Parliament and the Council, *Regulation (EU) No 517/2014 on fluorinated greenhouse gases*, OJL 150 (2014-05-04), pp. 195–230.
- [3] M. Abbrescia et al., *Eco-friendly gas mixtures for Resistive Plate Chambers based on tetrafluoropropene and helium*, Journal of Instrumentation, 11(08):P08019, 2016.
- [4] R. Guida, M. Caprì-Garrido, and B. Mandelli, *Characterization of RPC operation with new environmental friendly mixtures for LHC application and beyond*, Journal of Instrumentation, 11(07):C07016, 2016
- [5] B. Liberti et al., *Further gas mixtures with low environment impact*, Journal of Instrumentation, 11(09):C09012, 2016.
- [6] A. Bianchi, *R&D studies on eco-friendly gas mixtures for the ALICE Muon Identifier*, Journal of Instrumentation, 14(09):C09003, 2019.
- [7] IPCC Climate, The physical science basis, *Contribution of working group I to the Fifth Assessment Report of the Intergovernmental Panel on Climate Change*, 2014
- [8] M.S. Javadi et al., *Atmospheric chemistry of trans-CF₃CH=CHF: products and mechanisms of hydroxyl radical and chlorine atom initiated oxidation*, Atmospheric Chemistry and Physics, 8(12):3141–3147, 2008
- [9] ALICE collaboration et al., *ALICE Dimuon Forward Spectrometer: Technical Design Report*, CERN-LHCC-99-022, 1999
- [10] R. Arnaldi et al., *The ALICE Dimuon Trigger: overview and electronics prototypes*, Nuclear Instruments and Methods in Physics Research Section A, 456(1-2):126–131, 2000
- [11] A. Bianchi et al., *Characterization of tetrafluoropropene-based gas mixtures for the Resistive Plate Chambers of the ALICE Muon Spectrometer*, Journal of Instrumentation, 14(11):P11014, 2019
- [12] R. Arnaldi et al., *A low-resistivity RPC for the ALICE dimuon arm*, Nuclear Instruments and Methods in Physics Research Section A451.2 (2000), pp. 462–473.

- [13] R. Arnaldi et al, *Beam and ageing tests with a highly-saturated avalanche gas mixture for the ALICE p-p data taking*, Nuclear Physics B - Proceedings Supplements 158 (2006), pp. 149–153.
- [14] R. Arnaldi et al, *Influence of temperature and humidity on bakelite resistivity*, Nuclear Instruments and Methods in Physics Research Section A456.1–2 (2000), pp. 140–142.
- [15] R. Arnaldi et al, *Ageing tests on the low-resistivity RPC for the ALICE dimuon arm*, Nuclear Instruments and Methods in Physics Research Section A508 (2003), pp. 106–109.
- [16] P. Dupieux et al., *Upgrade of the ALICE Muon Trigger electronics*, Journal of Instrumentation 9.09 (2014): C09013.
- [17] M. Marchisone, *Performance of a Resistive Plate Chamber equipped with a new prototype of amplified front-end electronics in the ALICE detector*, Journal of Physics: Conference Series, Vol. 889. 1, IOP Publishing (2017), p. 012011.
- [18] F. Sauli, *Gaseous Radiation Detectors: fundamentals and applications*, Cambridge University Press, 2014.
- [19] L.G. Christophorou and J.K. Olthoff, *Electron attachment cross sections and negative ion states of SF₆*, International Journal of Mass Spectrometry, 205(1-3):27–41, 2001
- [20] P. Camarri, R. Cardarelli, A. Di Ciaccio, and R. Santonico, *Streamer suppression with SF₆ in RPCs operated in avalanche mode*, Nuclear Instruments and Methods in Physics Research Section A, 414(2-3):317–324, 1998
- [21] M. Capéans-Garrido et al., *A GIF++ Gamma Irradiation Facility at the SPS H4 Beam Line*, Technical report, 2009.