Estimation of absorbed dose in organs using Waza-AriV2 web-based software in head CT scans

Juan Miguel Lozano^{1,4,*}, H. Alejo-Martinez^{3,5}, Edison Salazar^{2,4}, and M.E. Castellanos⁵

¹Universidad del Valle, Physics department, Cali, Colombia

²Universidad del Valle, Radiodiagnostics Department, Cali, Colombia

³Hospital Universitario del Valle 'Evaristo García' E.S.E., Diagnostic Imaging Department, Cali, Colombia

⁴Clinica Imbanaco Grupo Quirónsalud, Diagnostic Imaging Department, Cali, Colombia

⁵Pontificia Universidad Javeriana, Medical Physics Program, Bogota, Colombia

*Lozano.juan@correounivalle.edu.co

ARISING FROM K. Yamashita et al. Nature. Scientific Reports, 11, 5435 (2021) doi:10.1038/s41598-021-85060-5 (2021).

Recently, Yamashita et al¹, reported direct measurements of ionizing radiation doses to individual organs in postmortem (using OSL dosimetry) that were exposed in the most frequent clinical CT scan protocols, corresponding to the whole body, head, thorax and abdomen. The authors¹ compare the experimental results with the values calculated in the Waza-AriV2 software^{2–4}, which is a system based on the monte carlo method that performs the estimation of organ doses from the exposure parameters used in the CT equipment. However, the results of the absorbed doses calculated in each examination had significant differences with respect to the doses measured directly in postmortem. In this communication, we made a calculation under the correct interpretation in one of the acquisition parameters which leads to a significant discrepancy between the estimated and measured values reported by Yamashita et al. We also make the comparison between the Waza-AriV2²⁻⁴ and NCICT⁵ software.

The effective dose of radiation received by patients undergoing diagnostic CT examinations can be classified in the zone of low absorbed doses⁶. On the other hand, the effective dose is associated with the relative risk of radiation exposure for the entire population, however, caution should be exercised when estimating individual radiological risk from this magnitude. The absorbed dose in organs is more associated with the estimation of individual risk⁷. Direct dose measurements in individual organs, in six postmortem exposed in different clinical CT scan protocols, were performed by Yamashita et al¹. The authors reported the exposure parameters of the CT scans carried out in a SOMATOM Emotion 16-slice (SIEMENS) and the average dose values in individual organs. These measured values were compared with those calculated with the software Waza-AriV2²⁻⁴, which performs a dose estimation in organs based on the monte carlo method using computational anthropomorphic phantoms according to the parameters of the CT scan. The absorbed doses calculated

with the software were significantly different from those reported experimentally, in particular, in the head examinations. The absorbed dose measured in the brain for the head CT scan was 31.18 mGy, while the calculated one was 123.31 mGy, the absorbed dose measured in the lens was 29.95 mGy, being the estimated equal to 117.2 mGy, which corresponds to a relative difference of 295.5% and 291.3%, respectively. This has some important implications because according to reports from the United States, approximately half of the collective effective dose administered by imaging procedures is due to CT studies⁸. Some studies suggest that repeated CT exposures to head, neck, and sinus are related to an increased risk of cataracts^{9,10}. The ICRP has published threshold dose values for detectable lens opacities of 0.5 Sv for acute or prolonged exposures¹¹. In this way, for patients who receive multiple CT studies, the accumulated lens doses could be of the order and even exceed the said threshold. Other studies¹² have shown that organ dose calculation software is increasingly used in dose tracking. In a comparative study of four available software, it was found that all were within 35% of variation with respect to the doses in organs that are inside the scan region¹³. For this reason, the significant differences found in the experimental results published by K. Yamashita et al^1 , could lead to an overestimation or underestimation of the dose in organs, and, therefore, an increase in the uncertainty when estimating the risk of the radiological effects.

The radiation dose in patients undergoing CT examinations is determined by parameters related to the equipment. Among them are beam filtration, beam collimation, detector configuration, image acquisition mode, kV, tube current, rotation time, slice thickness, pitch, and so forth. The charge on the x-ray tube in a CT is an exposure parameter that is defined as the product of the current in the x-ray tube (in units of milliamperes, mA) and the rotation time of the tube (in seconds, s). With the arrival of multislice scanners, some manufacturers (including Siemens) introduced an additional parameter called the effective mAs defined as:

$$mAs_{eff} = \frac{mAs}{pitch},\tag{1}$$

where the pitch relates the advance of the table per rotation to the total width of the collimated beam.

In the CT Siemens equipment, the mAseff is displayed on the CT operator console during scan parameter setup and postscan, as seen in Figure 1a. Organ dose calculation software requires the choice of the computational phantom that best represents the patient and the type of CT, as well as the information of the scan parameters configured during the study. In the 'table 1' reported by Yamashita et al¹, they present the irradiation conditions in the CT protocols, the tube current is mentioned in units of mAs, this unit does not correspond to the tube current (mA). In order to understand the parameters used and reproduce the absorbed doses in organs reported by the authors¹ using waza-ariV 2^{2-4} , we first took a sample of 20 patients from our institutions in a weight range similar to those of the study in question (between 50 and 60 kg) that were exposed to head CT scans on a SOMATOM Scope 16-slice (SIEMENS) and a Somatom Go Now 16-slice (SIEMENS) under the same parameters reported by K. Yamashita et al¹. Siemens Medical Solutions uses a current modulation system called CAREDose4D, which performs angular and longitudinal current modulation, adapted to different patient sizes and anatomical regions, for which the mAseff of each study displayed on the console corresponds to an average mAs_{eff} of all acquisitions (figure 1a). The current modulation in the

tube is carried out based on a reference value of mAs (mAs_{ref}) selected by the user according to the anatomy of the patient. In the sample of selected patients, the average mAs_{eff} of all the studies was 215 mAs, which is close to the value reported by Yamashita et al¹ in the 'table 1' for head scans, which was 220 mAs. In this way, we intuit that the value entered in the software, for the calculation of organ doses, is the mAs_{eff} instead of tube current (in units of mA).

If we carry out the respective correction, calculating the real value of the tube current from equation (1) we have that

$$mA = \frac{mAs_{eff} \times pitch}{t_r},$$
(2)

where t_r corresponds to the rotation time of the tube.


Yamashita et al¹, mention that none of the reduction techniques was carried out, including current modulation (no CareDose4D), therefore the tube current must be constant. For the head protocol, the authors reported a rotation time of 1.5 s and a pitch of 0.55, for which the value corresponding to the tube current (80.67 mA) was obtained from equation (2). This tube current is close to the current displayed on the equipment screen for a specific acquisition in one of our patients, when the study images are reconstructed (figure 1b). This value is relevant to estimate the organ doses using the monte carlo software Waza-AriV2²⁻⁴ and is shown in 'table 2' by K. Yamashita et al¹, for the head scan protocol. Using the same parameters of the said table, in which the values that we supply to the software Waza-AriV 2^{2-4} can be seen in table 2, We replicate the results shown in the 'table 3' of the K. Yamashita et al¹ publication; these results can be seen in table 3.

Head scan				
Tube voltage (kV)	Effective mAs/ Ref	Pitch factor	Beam collimation (mm)	Rotation time (seconds)
130	212 / 220	0.55	16×0.6	1.5

Table 1. Default parameters in a CT scan Siemens Somatom Scope 16-silce with a scan length of 174mm in default head clinical protocol.

11-Feb-2021 17:0	13				
Sección: Médico examinado Técnico:	pr:				
mAs total 2092	DLP total 797 mGy*cm				
	Scan KV mAs / ref.	CTDIvol mGy	DLP mGy*cm	TI s	cSL mm
Posición del pacie	ente H-SP				
Topogram	1 80	0.05(S)	2.49	2.9	0.6
Topogram	2 80	0.06(S)	2.99	3.3	0.6
CRANEO	3 130 212 / 220	45.46(S)	791.87	1.5	1.2

(a) Dose display shown at the end of a Siemens CT Head scan

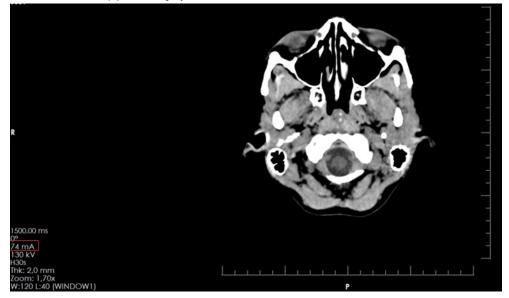

(b) Reconstructed image of the same CT scan study

Figure 1. (a) Dosimetric parameters displayed by the CT, the mAs shown is actually the effective mAs, /ref is the effective reference mAs from which the current will be modulated using the CareDose4D. (b) Reconstructed image of the same study (a) in which the value of the tube current in the z position corresponding to the acquisition shown can be observed in the lower left corner of the display (74 mA).

Head scan Waza-AriV2.				
Manufacturer/Scaner Model	Siemens	Emotion 16		
Filter	Head			
Tube Potential	130 kV			
Rotation Time	1.5 s			
Pitch Factor	0.55			
Beam width	16x0.6mm			
Gender	Male			
Phantom	Adult Optional Phantom			
Scan Type	Head Routine Head (helica			
Soon Dongo	Begin Position	1835 mm		
Scan Range	End Position	1675 mm		
AEC	Off			
Tube Current	220 mA			
Optional Phantom	On			
Height	158.9			
Weight	51.6			
CTDI Phantom Size	16cm			
SSDE	Off			

Table 2. Parameters given to the Waza-AriV2 web-based software to replicate the results obtained by K. Yamashita et al.

	Waza-AriV2	Reported Waza-AriV2	Difference
Organs	replicated organ dose	simulated Organ dose	between the two organ
	(mGy)	by K.Yamashita et al. (mGy)	doses (mGy)
Gonad	0	<0.01	<0.01
Prostate / uterus	0		
Urinary bladder	0		
Colon	0.01	<0.01	<0.01
Small intestine	0	<0.01	<0.01
Kidney	0.02	0.01	0.01
Pancreas	0.02		
Gall bladder	0.02		
Stomach	0.03		
Spleen	0.04		
Adrenals	0.03		
Liver	0.05	0.03	0.02
Heart	0.19		
Lungs	0.27	0.16	0.11
Breast	0.2		
Esophagus	0.36		
Thymus	0.3		
Thyroid	1.57	0.8	0.77
Salivary glands	33.67		
Oral cavity	15.56		
Out of Thorax	101.58		
Lens	122.75	117.2	5.55
Brain	132.57	123.31	9.26
Lymphaden	5.77		
Muscle	3.41		
Skin	10		
Bone	56.65		
Active marrow	8.39		

Table 3. Comparison between the simulated results obtained and the published results by K. Yamashita et al. Using the Waza-AriV2 software.

	Waza-AriV2	Postmortem	Difference
Organs	corrected organ dose	reported organ dose	between the two organ
	(mGy)	by K.Yamashita et al. (mGy)	doses (mGy)
Gonad	0	0.01 ± 0.0004	0.01 ± 0.0004
Prostate / uterus	0		
Urinary bladder	0		
Colon	0	0.05 ± 0.03	0.05 ± 0.03
Small intestine	0	0.05 ± 0.03	0.05 ± 0.03
Kidney	0.01	0.04 ± 0.03	0.03 ± 0.03
Pancreas	0.01		
Gall bladder	0.01		
Stomach	0.01		
Spleen	0.01		
Adrenals	0.01		
Liver	0.02	0.13 ± 0.09	0.11 ± 0.09
Heart	0.07		
Lungs	0.1	0.76 ± 0.9	0.66 ± 0.9
Breast	0.07		
Esophagus	0.13		
Thymus	0.11		
Thyroid	0.57	1.32 ± 0.70	0.75 ± 0.70
Salivary glands	12.33		
Oral cavity	5.7		
Out of Thorax	37.22		
Lens	44.97	29.95 ± 3.84	15.02 ± 3.84
Brain	48.57	31.18 ± 2.18	17.39 ± 2.18
Lymphaden	2.12		
Muscle	1.25		
Skin	3.66	Ŧ	Ť
Bone	20.75		
Active marrow	3.08		

Table 4. Comparison between the simulated results obtained with the corrected mA, using the Waza-AriV2 software and the published results by K. Yamashita et al. Measured in postmortem. † We did not consider the skin dose, because the postmortem measurements¹ were made only in the nipple and Umbilicus (outside the head scan region).

It was observed (table 3) that the replicated values of absorbed dose in organs obtained by the Waza-AriV2²⁻⁴ compared with the published results, differ in the main irradiated organs in 9.26 mGy (brain) and 5.55 mGy (lens), as well as differences less than 0.01 mGy in organs outside the scan region. Those variations compared with the values reported by K Yamashita et al¹, suggest that the tube current given in the software²⁻⁴ in order to estimate the organ doses corresponds to the effective mAs, value that is mentioned in 'table 1' reported by K. Yamashita et al¹. The small variations may be due to the fact that the exact parameters supplied to the software by the authors are unknown, a male virtual phantom was also chosen in contrast to the female one, chosen by the authors¹, under the argument that 2/3 of the total postmortem samples were males. On the other hand, the correction of the value of the tube current was done (80.67mA) from which we proceeded to estimate the organ doses, using the software²⁻⁴, these doses were compared with the values measured in postmortem reported by the authors K. Yamashita et al¹, these

findings were reported in table 4. The dose variations with the corrected tube current (mA) are of the same order as those measured by K Yamashita et al¹ in postmortem (giving a better approximation) with differences in the main irradiated organs of 15.02 ± 3.84 mGy (lens) and 17.39 ± 2.18 mGy (brain). Organ differences outside the scan region are less than 0.1 mGy. The differences between the measured values and those calculated from the software²⁻⁴ can be attributed to systematic errors induced by taking the average height and weight of various postmortems, without discrimination by gender, and to variations with respect to computational phantoms that have standard characteristics. This generates changes in the absorbed doses in organs calculated by the Waza-AriV2 software²⁻⁴. Additionally, the NCICT software⁵ was used to compare calculated doses (figure 2). The other CT scan protocols evaluated should also be reviewed following a similar methodology.

The preliminary results obtained show that the absorbed dose values calculated with the two software (figure 2) seem to overestimate the dose with respect to the postmortem measurements in the head scan, however, they represent a good

approximation in contrast to the results of Yamashita et al.¹. More detailed studies on individual postmortem dosimetry and the comparison of these doses with the different software should be carried out.

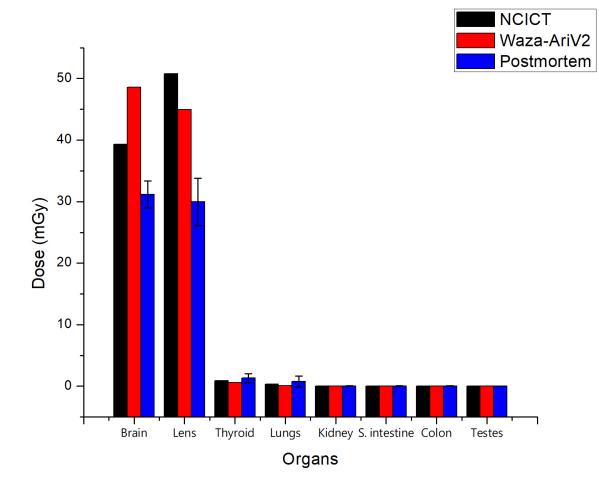


Figure 2. Comparison of dose estimation in organs in two software (NCICT & Waza-AriV2) and organ dose measured in postmortem reported by Yamashita et al.

Methods

We observed the effective mAs in the dose display of two CT's (Somatom Scope 16-slice, Somatom Go Now 16-slice (SIEMENS)) with the same parameters in twenty patients between 50 and 60 kg of our institutions to compared with the tube current reported by K. Yamashita et al¹. We also used the web-based software Waza-AriV2^{2–4} to replicate the data reported by K. Yamashita et al.¹ and the equation (2) from which we correct the value of the tube current. In addition we used the NCICT software⁵ to compared the reviewed results with the Waza-ariV2^{2–4} and the postmortem organ doses

reported by K. Yamashita et al.¹

Data availability

For our analyses, we used the 'Data of the table 1, Figure 4, and table 3 of K. Yamashita et al.¹' to replicate the data using the Waza-AriV2 web based software^{2–4} and the data of the table2. We also used the 'Data of the table 2, of K. Yamashita et al.¹' to compared the corrected tube current organ doses estimated with Waza-AriV2^{2–4} and the NCICT software⁵. Any other reasonable data requests should be addressed to J.M.L.

References

- Yamashita, K., Higashino, K. & Hayashi, H. e. a. Direct measurement of radiation exposure dose to individual organs during diagnostic computed tomography examination. *Sci Rep 11, 5435 (2021)*. https://doi.org/10.1038/ s41598-021-85060-5.
- 2. Takahashi, F. *et al.* Waza-ari: computational dosimetry system for x-ray ct examinations. i. radiation transport calculation for organ and tissue doses evaluation using jm phantom. *Prot. Dosimetry 146, 241–243 (2011).* https://doi.org/10.1093/rpd/ncr160.
- Ban, N. e. a. Waza-ari: computational dosimetry system for x-ray ct examinations ii: development of webbased system. *Radiat Prot Dosim.* 146, 244–247 (2011). https://doi.org/10.1093/rpd/ncr161.
- Ban, N. e. a. Development of a web-based ct dose calculator: Waza-ari. *Radiat. Prot. Dosim.* 147, 333–337 (2011). https://doi.org/10.1093/rpd/ncr333.
- Lee, C., Kim, K. P., Bolch, W. E., Moroz, B. E. & Folio., L. Ncict: a computational solution to estimate organ doses for pediatric and adult patients undergoing ct scans. 2015 J. Radiol. Prot. 35 891. https://doi.org/10. 1088/0952-4746/35/4/891.
- 6. on the Effects of Atomic Radiation., U. N. S. C. Sources, effects and risks of ionizing radiation: Unscear 2012 report to the general assembly with scientific annexes. *UN*; 2015, *Pag.* 23 ISBN:978-92-1-14307-5.
- J., M. C. Effective dose in medicine. annals of the icrp. Annals of the ICRP, 49(1 suppl), 126–140. (2020) https://doi.org/10.1177/0146645320927849.
- 8. (2019)., N. Medical radiation exposure of patients in the united states. *Report No. 184. Bethesda (MD): Na*-

tional Council on Radiation Protection and Measurements. Pag.6 ISBN:9781944888169.

- Yuan MK, T. D. *et al.* The risk of cataract associated with repeated head and neck ct studies: a nation-wide population-based study. *JR Am J Roentgenol.* 2013 Sep;201(3):626-30. https://doi.org/10.2214/AJR.12. 9652.
- I, Z.-M., CL, C. & SP., W. Radiation dose to the lens of eye and thyroid gland in paranasal sinus multislice ct. *Br J Radiol. 2003 Jun;76(906):418-20.* https: //doi.org/10.1259/bjr/82798696.
- FA, S., AV, A. & Hauer-Jensen M, e. a. Icrp publication 118: Icrp statement on tissue reactions and early and late effects of radiation in normal tissues and organs threshold doses for tissue reactions in a radiation protection context. *Annals of the ICRP. 2012;41(1-2):1-322.* https://doi.org/10.1016/j.icrp.2012.02.001.
- U, L., C, B., G, L.-J. & G., B. Dose reduction by automatic exposure control in multidetector computed tomography: comparison between measurement and calculation. *Eur Radiol.* 2009 Apr;19(4):1027-34. https://doi.org/10.1007/s00330-008-1204-6.
- De Mattia, C., Campanaro, F. & Rottoli, F. e. a. Patient organ and effective dose estimation in ct: comparison of four software applications. *Eur Radiol Exp 4, 14 (2020)*. https://doi.org/10.1186/s41747-019-0130-5.

Author contributions statement

J.M.L., H.A.M and E.S. contributed equally to this work. M.E.C provided Comments and approved the final work.

Competing interests

The authors declare no competing interests.