

Limits to the sensitivity of a rare-earth-enabled cryogenic vibration sensor

Anne Louchet-Chauvet¹ and Thierry Chanelière²

¹ESPCI Paris, Université PSL, CNRS, Institut Langevin, 75005 Paris, France

²Univ. Grenoble Alpes, CNRS, Grenoble INP, Institut Néel, 38000 Grenoble, France

(Dated: 8 December 2021)

Cryogenics is a pivotal aspect in the development of quantum technologies. Closed-cycle devices have recently emerged as an environmentally friendly and low-maintenance alternative to liquid helium cryostats. Yet the larger level of vibrations in dry cryocoolers forbids their use in most sensitive applications. In a recent work, we have proposed a broadband, contactless sensor based on the piezospectroscopic effect, *ie* the natural sensitivity of optical lines to strain exhibited by impurities in solids. This sensor builds on the exceptional spectroscopic properties of rare earth ions and operates below 4 K, where spectral hole burning considerably enhances the sensitivity. In this paper, we investigate the fundamental and technical limitations of this vibration sensor by comparing a rigid sample attachment to cold stage of a pulse-tube cryocooler and a custom-designed exchange gas chamber for acoustic isolation.

I. INTRODUCTION

The recent global effervescence around quantum technologies has led to an increasing need for reliable and efficient cryogenic systems. Continuously-operated closed-cycle cryocoolers are progressively replacing liquid helium cryostats that suffer from heavy logistics and high costs¹. However the low running cost and ease of use of dry systems comes at the price of a high level of acoustic vibrations generated by the cycling gas flow. These vibrations are problematic for many cryogenic experiments, including cavity QED², trapped ions spectroscopy³, quantum memories⁴ and frequency references based on rare-earth ions in crystals^{5,6}, scanning probe microscopy⁷, but also in the field of astronomy with bolometers⁸ or gravitational waves detectors⁹.

Relevant diagnosis of the vibrations in a cryostat is a necessity to ensure correct operation of the experiment. The specifications provided by commercial suppliers often prove insufficient to assess the actual impact of vibrations on a given experiment, either because the actual setup mechanical assembly differs from the nominal configuration, or because the information is incomplete (often limited to low acoustic frequencies of the order or below 1 kHz and/or peak-to-peak values).

In a recent publication¹⁰ we have proposed an original optical vibration sensor design with a high-frequency range (up to 1 MHz). This relies on the piezospectroscopic effect in rare-earth doped solids. In this work we investigate the sensitivity of this method. To that end, we explore various vibrational environments with the help of a customized pulse-tube cryocooler.

II. MEASURING VIBRATIONS WITH A RARE-EARTH DOPED CRYSTAL

Due to the screening of the outer electronic shells, the $4f$ energy levels of a rare-earth ion embedded in a crystal exhibit narrow transitions whose position is mainly determined by the crystal field created by the surrounding ligands. Modifying the interatomic distance, e.g. in a static way by applying high pressure, is a convenient way to explore the crystal structure and the site symmetry^{11,12}. This sensitivity to

strain, also known as the piezospectroscopic effect¹³, translates into a sensitivity to vibrations that is generally considered as an obstacle to high resolution measurements in rare-earth-based systems, especially in closed-cycle cryocoolers⁹. For this reason, custom solutions have been developed to reduce the transmission of vibrations in such devices while still ensuring a good thermal contact^{5,6,14}.

We recently proposed to take advantage of the sensitivity of rare-earth-doped crystals to vibrations to provide a local measurement of the mechanical stability of a sample holder in a cryocooler¹⁰. The proposed method consists in attaching a rare-earth ion-doped crystal to the holder under test and measure in real time the transmission of a laser beam tuned to the center of a narrow spectral hole whose linewidth can be adjusted from few tens of kHz to few MHz. The strain created by the vibrations leads to a time-dependent broadening of the hole, resulting in a variation of the hole depth.

More specifically, assuming a conservation of the spectral hole area, the transmission at the center of the hole is linked to the instantaneous atomic velocity of the rare-earth ions via the following relationship:

$$\kappa \frac{E}{\mathcal{V}} |\dot{x}(t)| = \frac{\alpha(t)}{\alpha_0 - \alpha(t)} \Gamma_{\text{HB}} \quad (1)$$

where κ is the piezospectroscopic sensitivity (expressed in Hz/Pa), E is the Young modulus of YAG, \mathcal{V} is the sound velocity in YAG. $\alpha(t)$ is the time-dependent crystal absorption at the center of the spectral hole, α_0 is the spectral hole depth. Γ_{HB} , the width of the spectral hole, is periodically measured by chirping the laser around the central frequency every 30 ms.

III. VIBRATION MEASUREMENT SENSITIVITY

A. Optical setup

The laser is a sub-kHz linewidth extended cavity diode laser (ECDL)¹⁵, tuned to the center of the Tm:YAG $^3H_6 \rightarrow ^3H_4$ line (793.37 nm). It is installed on a separate optical table to avoid coupling to the cryocooler vibrations. The cryostat is equipped with optical windows so we focus the laser beam

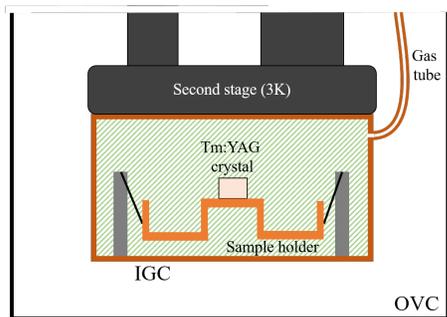


FIG. 1. Schematic cryostat cold part in configurations (b) and (c): the holder is suspended to the posts and the IGC is filled with helium gas. In configuration (a) the sample holder rests at the bottom of the IGC. (OVC: outer vacuum chamber. IGC: inner gas chamber.). The IGC and OVC are equipped with optical windows (not shown). A copper radiation shield (wrapped with multi-layer insulation), not represented for simplicity, is attached to the first stage.

in the crystal ($100\mu\text{m}$ waist). We collect the transmitted part that is measured with an avalanche photodetector (Thorlabs APD110A). For more detail on the experimental setup, the reader is referred to¹⁰.

B. Cryocooler design

We use a modified pulse-tube cryocooler TransMIT PTD-009 with an Oerlikon COOLPAK 2000A compressor. The modifications brought to the cryostat consist in an inner gas chamber (IGC) made of OFHC copper, attached to the cold finger. This chamber is equipped with two windows. It may optionally be filled with gas via a thin tube connected to a room temperature helium gas tank. The stainless steel injection tube is thermalized at the first stage of the cryocooler using a copper clamp and braids. Optimized design of the tube thickness (0.1mm for a 3.2mm diameter) and length (1.5m) ensures a negligible thermal load on both first and second stages. The crystal is thermally and mechanically contacted with an OFHC sample holder placed inside the IGC (see also Figure 5 for schematic 3D-visualisation). Even if the crystal itself can be thermally cooled by the exchange gas that will fill the IGC, its small surface (few tens of mm^2) would strongly limit the sample direct cooling. The suspended sample holder with a much larger surface (few tens of cm^2) is contrariwise efficiently cooled by the exchange gas.

Three experimental configurations are investigated in order to explore different vibrational environments for our sensor. In configuration (a), the sample holder is resting at the bottom of the IGC, with a thin layer of thermal grease to ensure good thermal contact and rigid mechanical coupling. The IGC and the tube are under vacuum. In this configuration the pulse tube vibrations are expected to couple efficiently to the crystal. In configurations (b) and (c), the sample holder is suspended by nylon threads to three stainless steel posts attached to the bottom of the IGC (see Figure 1). Such a suspension system is expected to significantly damp the vibrations transmitted to

#	mechanical contact	compressor
(a)	rigid	on
(b)	suspension in gas	on
(c)	suspension in gas	off

TABLE I. Experimental configurations allowing the exploration of three vibrational environments in the cryocooler.

the sample, similarly to the vibration isolation techniques developed for gravitational detectors¹⁶. Helium gas is admitted through the tube to reach a pressure around 100 mbar, ensuring thermalization of the sample holder on which the crystal is contacted. In configuration (b), the compressor is on, generating mechanical vibrations that are attenuated through the suspension threads and the gas. In configuration (c), the compressor is switched off for just a few seconds so that the sample temperature does not rise by more than 0.5 K. The three configurations are summarized in Table I.

We additionally monitor the acoustic environment up to 20 kHz with the help of a commercial soundmeter (RadioShack 33-099) attached to the outer cold head case of the cryostat. This device records the acoustic environment in the laboratory.

C. Spectral hole shapes

We first examine the spectral hole profile evolution in the three cryostat configurations, displayed in Figure 2, together with the audio signal recorded with the soundmeter. For configuration (a) we observe periodic variations of the spectral hole width, between 150 and 450 kHz, in synchrony with the rotary valve cycle. For configurations (b) and (c) however, both datasets reveal very stable and narrow spectral holes, with no visible effect of the rotary valve cycle on the hole shape and width. The average hole width is 30 kHz. This figure is remarkably low compared to the usual hole widths previously measured in Tm:YAG around 2-3 K with sub-kHz linewidth lasers and liquid helium cryostats (between 200 kHz and 400 kHz^{17,18}) and in Tm-doped crystals in general¹⁹⁻²¹. This result confirms the efficiency of the thermalization via the helium gas, together with the efficient vibration decoupling. This also suggests that wet cryostats actually provide a not so quiet acoustic environment (helium turbulence) leading to a broadening of the spectral hole.

D. Vibration measurements

Now we apply our measurement method to the three vibrational configurations (a) (b) and (c). Based on the pump beam transmitted power over a duration T , we record the crystal absorption coefficient $\alpha(t)$ and we use Eq. 1 to derive the atomic velocity and infer the corresponding vibration-driven displacement. The single-sided displacement spectral density

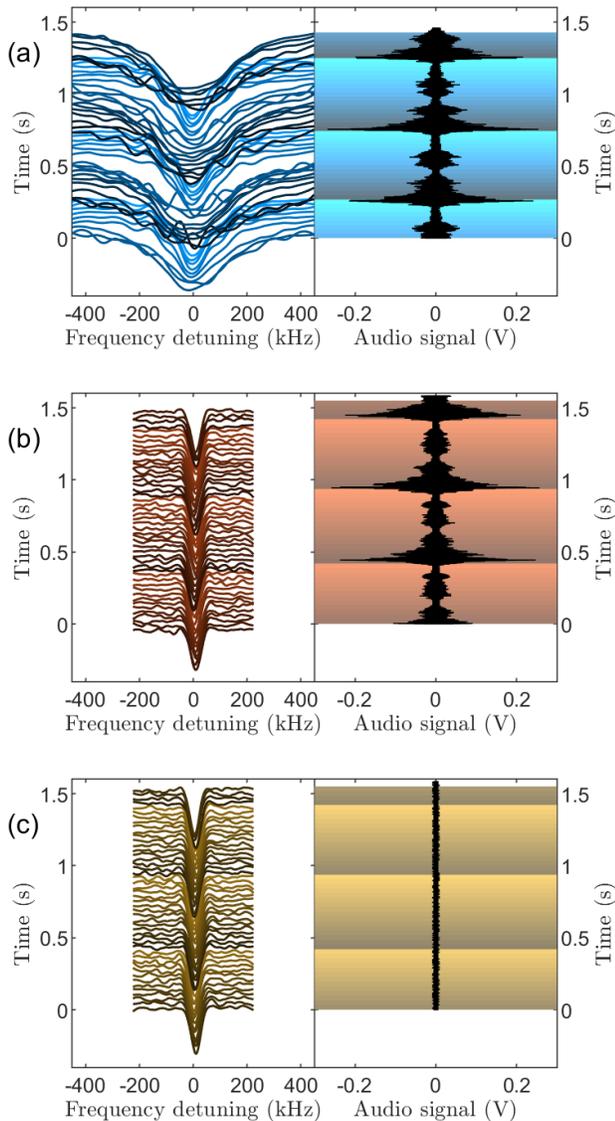


FIG. 2. Left: Spectral hole absorption throughout a repetition of 3 cycles (0.5s duration) of the rotary valve in configuration (a), (b) and (c) (see Table I). The graphs are vertically offset for a clear view of the spectral hole shape evolution. Right: Spectral hole width (red triangles) and audio signal simultaneously recorded (black line). Each moment in the valve cycle is identified with a color gradient (from dark at the beginning to bright at the end).

is expressed in $\text{m}/\sqrt{\text{Hz}}$ and is defined as:

$$A_x(f) = \sqrt{\frac{2}{T}} |\tilde{x}(f)| \quad (2)$$

where \sim denotes the Fourier transform. Equation 2 can also be written as a function of the atomic velocity, the relevant observable in our case (see Eq. 1):

$$A_x(f) = \sqrt{\frac{2}{T}} \frac{1}{2\pi f} |\tilde{x}(f)| \quad (3)$$

We carry out a quasi-continuous acquisition of the crystal transmission over a 1.5 s time interval (corresponding to 3 rotary valve cycles). The acquisition is interrupted 1 ms every 30 ms to measure the spectral hole width Γ_{HB} . On each 30 ms interval, we convert the crystal absorption $\alpha(t)$ into the atomic velocity $\dot{x}(t)$ following Equation 1, using the corresponding value of Γ_{HB} . Despite the periodic interruption, the high acquisition duty cycle (97%) allows us to concatenate the data and derive the displacement spectral density. We do this for the three vibrational configurations and present the results in Figure 3. We also plot the corresponding acoustic signal spectral density as measured by the soundmeter in Figure 4.

In configuration (a) the vibration spectrum exhibits an overall behaviour close to $1/f$. A large number of peaks is observed between 150 Hz and 200 kHz that we attribute to the vibrations of the rotary valve transmitted to the crystal via the rigid assembly.

In configuration (b), the vibration spectrum drops significantly over a broad frequency range from 1 Hz to 200 kHz, although the audio spectrum is unchanged, indicating an efficient vibration decoupling provided by the suspension. Only in the 50 – 400 Hz range does one observe an increase in the displacement spectral density in configurations (b) and (c), in the form of a series of peaks. We interpret these peaks as the result of a filtering of the acoustic noise by the 2 cm-long suspension wires whose eigenfrequency is of the order of 100 Hz.

The vibration spectrum in configuration (c) is identical to that of configuration (b), although the acoustic environment in the lab is much quieter especially in the 2 – 20 kHz (see Figure 4). This acoustic environment still contains significant contributions from other lab devices nearby that may propagate to the crystal via the helium gas or the suspension wires. Specifically we observe a few remaining peaks at 17 kHz, 20 kHz, 42 kHz and 122 kHz and their harmonics in the vibration spectra (b) and (c). These frequencies are compatible with the eigenfrequencies of low-order drum modes of the sample holder circular center platform (see Figure 5). Besides, these peaks are also present in the vibration spectrum obtained in configuration (a). This is why we interpret them as due to the residual vibrations (non cryocooler-related), filtered by the sample holder mechanical resonances.

The invariance of the atomic displacement spectral density with respect to the operation of the compressor shows that we have reached the background sensitivity for our vibration sensing method. We will now investigate the various mechanisms that contribute to this background.

E. Limits to the sensitivity

In order to make apparent the various sources of noise, we linearize Equation 1, assuming that the spectral hole shape is only marginally affected by the vibrations ($\alpha(t) \ll \alpha_0$):

$$|\dot{x}(t)| = \frac{\gamma}{\kappa E} \Gamma_{\text{HB}} \frac{\alpha(t)}{\alpha_0} \quad (4)$$

The absorption coefficient is derived from the crystal transmission by using the Bouguer-Beer-Lambert absorption law

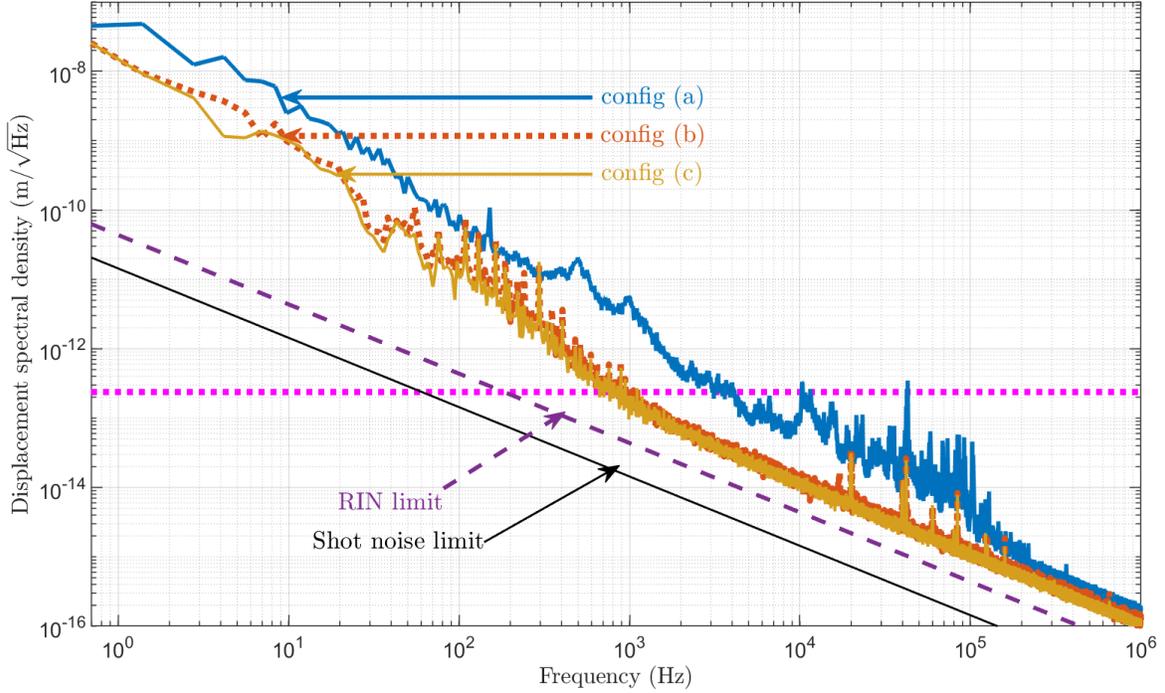


FIG. 3. Single-sided displacement spectral density obtained with our vibration sensor for the three configurations (a) (b) and (c) (see Table I). Each spectrum represents the vibrations measured over three rotary valve cycles (≈ 1.5 s). Dashed purple line: sensitivity limit due to the laser relative intensity noise (RIN). Solid black line: sensitivity limit due to the laser shot noise. Pink horizontal line: shot-noise limit that would apply for an interferometric measurement with a similar optical power.

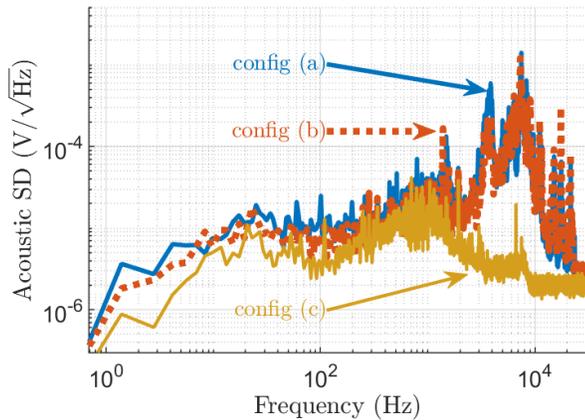


FIG. 4. Audio spectral density as measured by the soundmeter in contact with the rotary valve. In configurations (a) and (b), the sound sample reveals a dominating contribution of the cryocooler to the lab acoustic environment. In configuration (c) when the cryocooler is switched off, the remaining lab equipment can distinctly be heard, notably the turbomolecular vacuum pump (Pfeiffer HiCube80).

linking the transmitted photon rate $I(t)$ to the incoming photon rate I_0 : $I(t) = I_0 e^{-\alpha(t)L}$. Based on the fact that $\alpha_0 L$ is of

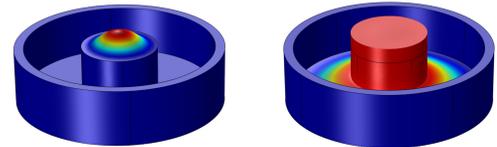


FIG. 5. Lowest order vibration modes for the sample holder. A COMSOL Multiphysics simulation gives an eigenfrequency of 70 kHz and 7 kHz for the (0, 1) drum mode for the center and outer platform, respectively from left to right.

the order of unity, we obtain:

$$|\dot{x}(t)| = \frac{\mathcal{V}}{\kappa E} \frac{\Gamma_{\text{HB}}}{\alpha_0 L} \left(1 - \frac{I(t)}{I_0} \right) \quad (5)$$

The displacement spectral density can therefore be written as:

$$A_x(f) = \frac{1}{2\pi f} \frac{\mathcal{V}}{\kappa E} \frac{\Gamma_{\text{HB}}}{\alpha_0 L} \underbrace{\frac{A_I(f)}{I_0}}_{\sqrt{\text{RIN}}} \quad (6)$$

In this expression the parameters Γ_{HB} and $\alpha_0 L$ are measured experimentally. The ratio $\frac{A_I(f)}{I_0}$ corresponds to the square root of the laser relative intensity noise (RIN). We estimate the

relative intensity noise of our ECDL laser by an independent measurement with a similar power: $\left. \frac{A_I(f)}{I_0} \right|_{\text{RIN}} = 2.5 \times 10^{-6}/\sqrt{\text{Hz}}$. Using Equation 6 we derive an estimation of the RIN-limited sensitivity floor for our displacement measurement, taking $\alpha_0 L = 1$ and $\Gamma_{\text{HB}} = 300$ kHz, a typical spectral hole width measured in configuration (a) during the noisy phase of the rotary valve cycle [see Figure 2(a)]:

$$A_x^{\text{RIN}}(f) = \frac{4.4}{f} \times 10^{-11} \text{ m}/\sqrt{\text{Hz}} \quad (7)$$

and plot it as a dashed purple line in Figure 3.

The laser RIN is a technical issue, ultimately limited by the laser intensity shot noise $\left. \frac{A_I(f)}{I_0} \right|_{\text{shot}} = \sqrt{\frac{2}{I_0}}$ where I_0 is the photon rate. Considering the typical laser power collected on the detector in the present work (0.7 μW), this contribution amounts to $8.3 \times 10^{-7}/\sqrt{\text{Hz}}$. Again, using Equation 6 we obtain a fundamental limit for the piezospectroscopic vibration measurement:

$$A_x^{\text{shot}}(f) = \frac{1.4}{f} \times 10^{-11} \text{ m}/\sqrt{\text{Hz}} \quad (8)$$

This limit is represented as a black line in Figure 3. One should bear in mind that this shot noise limit is affected by a $\Gamma_{\text{HB}}/\alpha_0 L$ scaling factor (see Eq. 6). While the spectral hole width Γ_{HB} is ultimately limited by twice the homogeneous linewidth ($\Gamma_{\text{HB}} \geq 2\Gamma_h = 6$ kHz in Tm:YAG²²), reaching such a low limit would require both a very low vibration level and a reduced laser irradiance on the crystal to avoid optical saturation, in turn leading to a reduced hole depth α_0 .

Another noise source that could lead to a contribution to the vibration background is the laser frequency noise. However, since the pump beam mean frequency is by essence centered on the spectral hole, the laser frequency noise only contributes to second order. Still, the laser jitter on the timescale of the hole lifetime impacts the spectral hole width Γ_{HB} and therefore globally affects the sensitivity, but as a scaling factor (see Eq. 4).

Overall, we have identified the sensitivity limits of our vibration sensor. Even in the quietest vibrational configuration, the remaining acoustic perturbations transmitted to the crystal lead to a series of peaks that limit the sensitivity below 1 kHz. At higher frequencies, the sensor sensitivity reaches a $1/f$ floor limited by the laser intensity noise. This latter in our case is an order of magnitude larger than the fundamental shot noise limit.

IV. DISCUSSION

Our piezospectroscopic vibration sensor fundamentally differs from conventional optical methods (*ie*, interferometric) because its sensitivity is based on strain (and not on position). This is why the sensitivity increases with the frequency. In this work we have reached 1 MHz but this is a mere technical limitation given by the 2 MHz sampling rate. More specifically, we demonstrate a 10^{-16} m/ $\sqrt{\text{Hz}}$ background displacement

sensitivity at 1 MHz with a 0.7 μW optical power, whereas its counterpart in an interferometric measurement would only reach $\frac{\lambda}{2\sqrt{I_0}} = 2.4 \times 10^{-13}$ m/ $\sqrt{\text{Hz}}$ with the same power. This interferometric measurement sensitivity is displayed in Figure 3. Reaching the sensitivity of our piezospectroscopic method at 1 MHz with an interferometric setup would require working with an interferometer with a high finesse (> 1000).

Besides sensitivity, we point out that our method allows for inertial sensing, unlike conventional optical methods that give access to the displacement with respect to a reference point, which could itself be unstable. This property is also a direct consequence of the strain-coupling mechanism of our sensor. This is a decisive asset of our method for the most vibration-sensitive setups, including those using micro or nano-mechanical resonators, where inertial stability is required.

V. CONCLUSION

In a previous publication¹⁰ we have proposed an original inertial method to probe acoustic vibrations in a cryogenic environment on a wide frequency range, based on spectral hole-burning in a rare-earth ion-doped crystal. In the present work we have investigated the technical and fundamental limits of this method. This was made possible by exploring various vibrational configurations in a pulse-tube cryocooler. In the quietest environment combining mechanical decoupling from the cold finger and momentary pause of cryocooler operation, we have observed the narrowest spectral holes ever reported in a Tm:YAG crystal. Above 1 kHz we have reached a $1/f$ background floor that we ascribe to laser intensity noise. Below 1 kHz, the excess of noise is attributed to the remainder of the strongly attenuated mechanical vibrations transmitted to the crystal by the suspension and the helium gas, characterizing the limit of our vibration-decoupling setup.

VI. ACKNOWLEDGMENTS

The authors acknowledge support from the French National Research Agency (ANR) projects ATRAP (ANR-19-CE24-0008), and MIRESPIN (ANR-19-CE47-0011), and the LABEX WIFI (Laboratory of Excellence within the French Program "Investments for the Future") under references ANR-10-LABX-24 and ANR-10-IDEX-0001-02 PSL*.

¹D. Kramer, "Helium shortage has ended, at least for now," *Physics Today* **5** (2020).

²S. Vadia, J. Scherzer, H. Thierschmann, C. Schäfermeier, C. D. Savio, T. Taniguchi, K. Watanabe, D. Hunger, K. Karraï, and A. Högele, "Open-cavity in closed-cycle cryostat as a quantum optics platform," arXiv preprint arXiv:2103.05619 (2021).

³P. Mücke, J. Stark, S. King, T. Leopold, T. Pfeifer, L. Schmoeger, M. Schwarz, L. Spieß, P. Schmidt, and J. Crespo López-Urrutia, "Closed-cycle, low-vibration 4 K cryostat for ion traps and other applications," *Review of Scientific Instruments* **90**, 065104 (2019).

⁴M. Gündoğan, P. M. Ledingham, K. Kutluer, M. Mazzera, and H. De Riedmatten, "Solid state spin-wave quantum memory for time-bin qubits," *Physical Review Letters* **114**, 230501 (2015).

- ⁵M. J. Thorpe, D. R. Leibbrandt, and T. Rosenband, “Shifts of optical frequency references based on spectral-hole burning in $\text{Eu}^{3+}:\text{Y}_2\text{SiO}_5$,” *New Journal of Physics* **15**, 033006 (2013).
- ⁶O. Gobron, K. Jung, N. Galland, K. Predehl, R. Le Targat, A. Ferrier, P. Goldner, S. Seidelin, and Y. Le Coq, “Dispersive heterodyne probing method for laser frequency stabilization based on spectral hole burning in rare-earth doped crystals,” *Optics Express* **25**, 15539–15548 (2017).
- ⁷F. P. Quacquarelli, J. Puebla, T. Scheler, D. Andres, C. Bödefeld, B. Sips, C. Dal Savio, A. Bauer, C. Pfeleiderer, A. Erb, and et al., “Scanning probe microscopy in an ultra-low vibration closed-cycle cryostat: Skyrmion lattice detection and tuning fork implementation,” *Microscopy Today* **23**, 12–17 (2015).
- ⁸R. Maisonobe, J. Billard, M. De Jesus, A. Juillard, D. Misiak, E. Olivieri, S. Sayah, and L. Vagneron, “Vibration decoupling system for massive bolometers in dry cryostats,” *Journal of Instrumentation* **13**, T08009 (2018).
- ⁹T. Tomaru, T. Suzuki, T. Haruyama, T. Shintomi, A. Yamamoto, T. Koyama, and R. Li, “Vibration analysis of cryocoolers,” *Cryogenics* **44**, 309–317 (2004).
- ¹⁰A. Louchet-Chauvet, R. Ahlefeldt, and T. Chanelière, “Piezospectroscopic measurement of high-frequency vibrations in a pulse-tube cryostat,” *Review of Scientific Instruments* **90**, 034901 (2019).
- ¹¹C. Bungenstock, T. Tröster, and W. Holzapfel, “Effect of pressure on free-ion and crystal-field parameters of Pr^{3+} in LOCl ($L = \text{La}, \text{Pr}, \text{Gd}$),” *Physical Review B* **62**, 7945 (2000).
- ¹²A. Kaminska, A. Kozanecki, M. Ramirez, L. Bausa, G. Boulon, M. Bettinelli, M. Boćkowski, and A. Suchocki, “Spectroscopic study of radiative intra-configurational $4f \rightarrow 4f$ transitions in Yb^{3+} -doped materials using high hydrostatic pressure,” *Journal of Luminescence* **169**, 507–515 (2016).
- ¹³A. Kaplyanskii, “Noncubic centers in cubic crystals and their piezospectroscopic investigation,” *Optics and Spectroscopy* **16**, 329 (1964).
- ¹⁴Y.-H. Chen, X. Fernandez-Gonzalvo, and J. J. Longdell, “Coupling erbium spins to a three-dimensional superconducting cavity at zero magnetic field,” *Physical Review B* **94**, 075117 (2016).
- ¹⁵V. Crozatier, F. De Sèze, L. Haals, F. Bretenaker, I. Lorgeré, and J.-L. Le Gouët, “Laser diode stabilisation for coherent driving of rare earth ions,” *Optics Communications* **241**, 203–213 (2004).
- ¹⁶T. Ushiba, T. Akutsu, S. Araki, R. Bajpai, D. Chen, K. Craig, Y. Enomoto, A. Hagiwara, S. Haino, Y. Inoue, *et al.*, “Cryogenic suspension design for a kilometer-scale gravitational-wave detector,” *Classical and Quantum Gravity* **38**, 085013 (2021).
- ¹⁷F. De Seze, A. Louchet, V. Crozatier, I. Lorgeré, F. Bretenaker, J.-L. Le Gouët, O. Guillot-Noël, and P. Goldner, “Experimental tailoring of a three-level Λ system in $\text{Tm}^{3+}:\text{YAG}$,” *Physical Review B* **73**, 085112 (2006).
- ¹⁸R. Lauro, T. Chanelière, and J.-L. Le Gouët, “Slow light using spectral hole burning in a Tm^{3+} -doped yttrium-aluminum-garnet crystal,” *Physical Review A* **79**, 063844 (2009).
- ¹⁹R. Macfarlane, “Spectral hole burning in the trivalent thulium ion,” *Optics Letters* **18**, 829–831 (1993).
- ²⁰C. Thiel, Y. Sun, T. Böttger, W. Babbitt, and R. Cone, “Optical decoherence and persistent spectral hole burning in $\text{Tm}^{3+}:\text{LiNbO}_3$,” *Journal of Luminescence* **130**, 1598–1602 (2010).
- ²¹C. W. Thiel, N. Sinclair, W. Tittel, and R. L. Cone, “ $\text{Tm}^{3+}:\text{Y}_3\text{Ga}_5\text{O}_{12}$ materials for spectrally multiplexed quantum memories,” *Physical Review Letters* **113**, 160501 (2014).
- ²²R. M. Macfarlane, “Photon-echo measurements on the trivalent thulium ion,” *Optics Letters* **18**, 1958–1960 (1993).