

# Interferometric mass spectrometry

Radu Ionicioiu

Horia Hulubei National Institute of Physics and Nuclear Engineering, 077125 Bucharest-Măgurele, Romania

Accelerator mass spectrometry (AMS) is a widely-used technique with multiple applications, including geology, molecular biology and archeology. Although extremely precise, AMS requires tandem accelerators and bulky magnets which confines it to large laboratories. Here we propose interferometric mass spectrometry (IMS), a novel method of mass separation which uses quantum interference. IMS employs the wave-like properties of the samples, and as such is complementary to AMS, in which samples are particle-like. This complementarity has two significant consequences: (i) in IMS separation is performed according to the absolute mass  $m$ , and not to the mass-to-charge ratio  $m/q$ , as in AMS; (ii) in IMS the samples are in the low-velocity regime, in contrast to the high-velocity regime used in AMS. Potential applications of IMS are compact devices for mobile applications, sensitive molecules that break at the acceleration stage and neutral samples which are difficult to ionise.

*Introduction.*— Mass spectrometry is a widespread tool with applications in several fields like chemistry, molecular biology, geology and archeology [1]. A well-known example is carbon dating, a technique used to determine the age of organic samples by measuring the relative abundances of  $^{12}\text{C}$  and  $^{14}\text{C}$  isotopes. Due to its precision and conceptual simplicity, carbon dating had a huge impact and revolutionised several fields like archeology, palaeontology and anthropology.

One of most precise techniques is accelerator mass spectroscopy (AMS). In AMS the samples (i.e., the mass species we want to separate) are first ionised, then accelerated to high velocities using a tandem accelerator. Electric and magnetic fields are used as velocity filters and to separate different mass species according to their mass-to-charge ratios  $m/q$ . After the separation stage, an array of particle detectors count the number of atoms for each species.

Since all samples are, after all, quantum systems, one question arises. Can we use the wave-like properties for mass separation? Here we answer this question in the affirmative. Quantum superposition and matter-wave interferometry have been experimentally demonstrated for electrons [2, 3], neutrons [4], atoms and increasingly large molecules [6], including C60 [7], molecules [8–10], molecular clusters [11] and polypeptides [12].

In this article we describe a novel mass spectrometry method which uses quantum interference as a mass-separation mechanism. Interferometric sorting has been used previously for spin separation [13], sorting quantum systems [14], orbital angular momentum of photons [15–17] and radial modes of light [18, 19]. We start with a brief overview of the the standard method, namely accelerator mass spectroscopy. We then introduce interferometric sorting, first for two mass species and then for the general case of  $N$  species.

*Accelerator mass spectrometry.*— The basic idea of a mass spectrometer is shown in Fig.1. The samples of masses  $m_i$  enter a mass separator which directs each mass species (isobars) into distinct spatial channels. Each channel  $i$  has a particle counter which registers the number of particles  $N_i$  for a given period of time. The mass spectrum is calculated from the relative counting frequencies  $N_1, N_2, \dots$ , where  $N_i$  is the number of particles in detector  $i$ , corresponding to mass  $m_i$ . The detectors themselves are mass-insensitive, i.e., they do

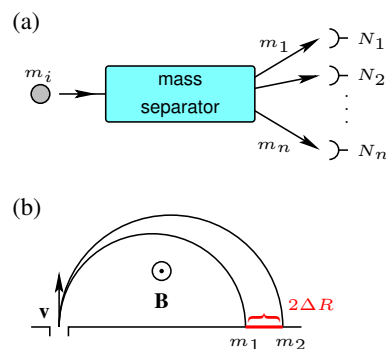


FIG. 1: (a) Schematics of a mass spectrometer. A mass analyser (separator) separates different mass species into distinct spatial channels; each channel has a particle counter measuring the number of particles  $N_i$ . (b) In AMS the analyser uses magnetic fields for mass separation.

not distinguish between different mass species. Thus the key element is the mass separator which sorts the particles into distinct spatial channels (paths) according to their masses.

In AMS the mass analyser (or separator) uses the Lorentz force acting on charged particles. From  $qvB = mv^2/R$ , we have

$$R = \frac{mv}{qB} \quad (1)$$

A velocity filter placed before the analyser ensures that all samples have the same velocity  $v$ . Consider two mass species  $(m_1, q_1)$  and  $(m_2, q_2)$ . Then the separation between the two species is  $2\Delta R$ , with

$$\Delta R = \frac{v}{B} \left( \frac{m_2}{q_2} - \frac{m_1}{q_1} \right) \quad (2)$$

There are two important points to note here. First, the Lorentz force separates species according to the mass-to-charge ratio  $m/q$ , and not to the mass  $m$ . Therefore the samples have to be electrically charged, as the Lorentz force cannot separate neutral particles. Second, for a given magnetic field  $B$  the separation between two samples is proportional to the velocity

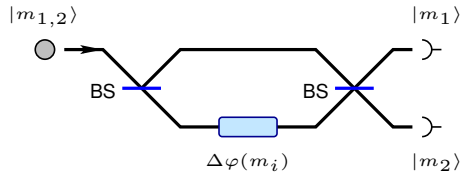


FIG. 2: Interferometric mass spectrometry (IMS) for two mass species. A Mach-Zehnder interferometer has a mass-dependent phase-shift  $\Delta\varphi(m_i) := \Delta\varphi_i$  in one arm, such that the mass species  $m_{1,2}$  acquire different phases  $\Delta\varphi_{1,2}$ . At the second beam-splitter  $m_1$  interferes constructively in output 1 and destructively in output 2, whereas  $m_2$  interferes constructively in output 2 and destructively in output 1.

$v$ . Thus, in order to increase the separation  $\Delta R$  for different mass species, we need to work in the high-velocity regime, hence to use TANDEM accelerators.

*Interferometric sorting: two mass species.*— Interferometric sorting uses wave-like properties of quantum systems (atoms, molecules, proteins etc) to separate the samples according to their mass. An interferometric mass separator uses constructive/destructive interference to separate different species  $m_i$  into distinct spatial channels (paths). First we discuss the simpler case of sorting two mass species, and then we generalise to  $N$  species.

Let us consider the problem of sorting two mass species  $m_1, m_2$ . The general scheme is shown in Figure 2. It consists of a Mach-Zehnder interferometer (MZI) with a mass-dependent phase shift in the lower arm:

$$|m_i\rangle \rightarrow e^{i\Delta\varphi_i} |m_i\rangle, \quad i = 1, 2 \quad (3)$$

To achieve (perfect) interferometric separation of the two mass species, we choose the phase shifts such that  $m_1$  has constructive interference in output 1, whereas  $m_2$  has constructive interference in output 2. This implies the phase-shift induces a phase  $\Delta\varphi_1 = 0$  for  $m_1$  and  $\Delta\varphi_2 = \pi$  for  $m_2$ :

$$\begin{aligned} |m_1\rangle &\rightarrow |m_1\rangle \\ |m_2\rangle &\rightarrow -|m_2\rangle \end{aligned} \quad (4)$$

In quantum information parlance, the mass-dependent phase-shift acts like a controlled- $Z$  gate between the mass and the path degrees of freedom [14]. Therefore the interferometer acts as a CNOT gate between mass and path degrees of freedom. This insight is important and will provide the solution to the general case of sorting  $N$  species. Next we discuss how to implement the mass-dependent phase shift.

**Mass-dependent phase shift.** Consider a quantum system (atom, molecule etc), incident on a Mach-Zehnder interferometer, Fig.2; we will use “particle” as a short-hand for quantum system. After the first beamsplitter, the particle is in superposition of being in the two paths. We assume the paths have lengths  $L_1$  and  $L_2$ , respectively. The particle interferes with itself at the second beamsplitter. The phase difference between the two paths is

$$\Delta\varphi = \frac{2\pi\Delta L}{\lambda} = \frac{2\pi\Delta L}{h}mv \quad (5)$$

with  $\Delta L = L_2 - L_1$ ;  $\lambda = h/mv$  is the de Broglie wavelength of the particle of mass  $m$  and velocity  $v$ .

Now suppose we have two mass species  $m_{1,2}$  entering the interferometer with velocities  $v_{1,2}$ , respectively. Then

$$\frac{\Delta\varphi_1}{\Delta\varphi_2} = \frac{m_1 v_1}{m_2 v_2} \quad (6)$$

To achieve *perfect interferometric sorting*, we design the interferometer such that  $m_1$  ( $m_2$ ) exits on output 1 (output 2) with unit probability. This implies the following relations:

$$\Delta\varphi_1 = 2k_1\pi \quad (7a)$$

$$\Delta\varphi_2 = (2k_2 + 1)\pi \quad (7b)$$

with arbitrary  $k_1, k_2 \in \mathbb{Z}$ . Thus the conditions for interferometric sorting are (not all equations are independent):

$$\frac{m_1 v_1}{m_2 v_2} = \frac{2k_1}{2k_2 + 1} \quad (8a)$$

$$\Delta L = k_1 \lambda_1 = k_1 \frac{h}{m_1 v_1} \quad (8b)$$

$$\Delta L = (k_2 + \frac{1}{2}) \lambda_2 = (k_2 + \frac{1}{2}) \frac{h}{m_2 v_2} \quad (8c)$$

We assume there is a velocity filter before the interferometer, hence  $v_1 = v_2 = v$  and the first equation becomes  $m_1/m_2 = 2k_1/(2k_2 + 1)$ .

Clearly, the parameter we need to control accurately is the path difference,  $\Delta L$  between the two arms. We can see this in the the next example.

**Example.** Carbon dating is a standard method to determine the age of organic materials like wood, bone etc. In carbon dating we measure the relative abundances of two carbon isotopes,  $^{12}\text{C}$  and  $^{14}\text{C}$ . We have  $m_1 = 1.99 \times 10^{-26}$  kg ( $^{12}\text{C}$ ) and  $m_1/m_2 = 6/7$ . This gives  $k_1 = k_2 = 3$  and  $\Delta L = 3\lambda_1$ . For  $v = v_{1,2} = 100$  m/s we obtain  $\Delta L \approx 1$  nm. If we slow down the samples to  $v = 1$  m/s, then  $\Delta L \approx 0.1$   $\mu\text{m}$ .

The challenge is to accurately control (and stabilise) the path difference  $\Delta L$  between the two arms of the MZI. Commercially available piezo-stages used for nano-positioning (e.g., in AFM) have sub-nanometer resolution  $\sim 0.3$  nm [20].

*Interferometric sorting:  $N$  mass species.*— We now turn to the general case. The problem of sorting quantum systems according to an arbitrary (discrete) degree of freedom has been studied in [14]. Here we apply similar consideration for sorting  $N$  mass species  $m_0, \dots, m_{N-1}$ .

The device for interferometric sorting is a multi-path Mach-Zehnder interferometer and consists of an input coupler, a waveguide array and an output coupler, Fig. 3. All mass species enter through the same port of the input coupler. The waveguide array has  $N$  waveguides of lengths  $L_0, \dots, L_{N-1}$ . The output coupler has  $N$  output waveguides used for sorting the  $N$  species. The input (output) coupler is a free-propagating region and implements the Fourier transform on spatial modes (paths) [21–23]. The input coupler ensures the quantum systems enter the waveguide array in an equal superposition of paths,  $\frac{1}{\sqrt{N}} \sum_{i=0}^{N-1} |i\rangle$ . At the output coupler all

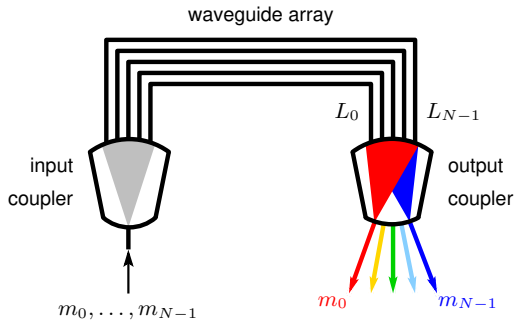


FIG. 3: Interferometric mass separation for  $N$  species.

the waves coming from the waveguide arrays interfere with different phases.

For sorting, we require that mass  $m_k$  exits from output port  $k$  with unit probability, i.e., there is constructive interference in port  $k$  and destructive interference in all other ports  $j \neq k$ . We assume that all species have the same velocity  $v$ , hence there is a velocity filter before the analyser. A species  $m_k$  propagating along waveguide  $L_s$  acquires a phase shift

$$\varphi_{k,s} = 2\pi \frac{L_s}{\lambda_k} \quad (9)$$

with  $\lambda_k = h/m_k v$  its de Broglie wavelength. Since species  $m_k$  exits on port  $k$  with probability  $p = 1$ , this requires the phase differences between each arm of the interferometer and the reference 0-th arm to satisfy the conditions [14]:

$$\Delta\varphi_{k,s} := \varphi_{k,s} - \varphi_{k,0} = \frac{2\pi}{N} ks + 2\pi n_{k,s} \quad (10)$$

for all  $k, s = 0, \dots, N-1$  and arbitrary integers  $n_{k,s} \in \mathbb{Z}$ ,  $n_{k,0} = 0$ . These are the conditions for *perfect interferometric sorting* which generalise eqs. (7a), (7b). We have

$$\Delta L_s := L_s - L_0 = \lambda_k \left[ \frac{ks}{N} + n_{k,s} \right] \quad (11)$$

$$= \frac{h}{m_k v} \left[ \frac{ks}{N} + n_{k,s} \right] \quad (12)$$

for all  $k, s = 0, \dots, N-1$  and arbitrary  $n_{k,s} \in \mathbb{Z}$ ,  $n_{k,0} = 0$ .

Experimentally we need to control the path differences  $\Delta L_s$  of the waveguide array in order to induce the appropriate phase-shifts. Since  $\Delta L_s \sim v^{-1}$ , this implies that we need to work in the low velocity regime.

From eq. (10) we see that, given a mass species  $m_k$ , all the phases  $\Delta\varphi_{k,s}$ ,  $s = 0, \dots, N-1$ , are different (modulo  $2\pi$ ) iff  $(k, N)$  are coprime. Consequently, if  $N$  is a prime number, all phases  $\Delta\varphi_{k,s}$  are distinct (mod  $2\pi$ ), for any mass species  $m_k$ ,  $k = 0, \dots, N-1$ .

*Errors.*— So far we have discussed the ideal case. We now briefly analyse the effect of errors around the ideal parameters. One source of errors are fluctuations in length of the waveguide array. We assume that path  $s$  of the interferometer has length  $L'_s = L_s + \delta L_s$ , where  $\delta L_s$  is the fluctuation

around the theoretical (ideal) value  $L_s$ . Thus species  $m_k$  propagating along path  $s$  acquires a phase  $\varphi'_{k,s} = \varphi_{k,s} + \delta\varphi_{k,s}$ , with  $\varphi_{k,s} = 2\pi L_s/\lambda_k$  and  $\delta\varphi_{k,s} = 2\pi\delta L_s/\lambda_k$ . For the mass species  $m_k$ , the phase difference between path  $s$  and path 0 is

$$\Delta\varphi'_{k,s} := \varphi'_{k,s} - \varphi'_{k,0} = \Delta\varphi_{k,s} + \frac{2\pi}{\lambda_k}(\delta L_s - \delta L_0) \quad (13)$$

Consequently, if all the paths fluctuate by the same amount,  $\delta L_s = \delta L_0, \forall s = 0, \dots, N-1$ , then the perfect sorting conditions (10) are unchanged. This shows the robustness under global fluctuations, where all paths are modified equally.

Consider now uncorrelated errors. For an  $N$ -path interferometer, the phases in eq. (10) are multiples of  $\delta\varphi = \frac{2\pi}{N}$ , which corresponds to a difference in path length

$$\delta L = \frac{\lambda}{N} \quad (14)$$

As a rule of thumb, for  $N$  species we need to control the path differences in the interferometer to order  $\mathcal{O}(\lambda/N)$ , with  $\lambda = \min_k \lambda_k$  the smallest wavelength of the set. One way around this is to concatenate a series of separation stages, where each stage separates only between a small number of species.

*Discussion and conclusions.*— It is insightful to compare interferometric mass spectrometry proposed here with the standard, widely-used accelerator mass spectrometry.

Conceptually, the two methods are complementary: in AMS samples are particle-like with localised, well-defined trajectories, while in IMS they have a wave-like behaviour with delocalised trajectories. More importantly, this duality also extends to the velocity regime. To achieve a high sensitivity, in AMS the samples are accelerated to high velocities. In contrast, IMS uses the low-velocity regime, corresponding to large  $\lambda$ . There are several differences between the two methods; these are summarised in Table I.

**Separation mechanism.** A crucial difference between AMS and IMS is the separation mechanism. AMS uses the Lorentz force  $q(\mathbf{E} + \mathbf{v} \times \mathbf{B})$  for separation. This has two implications: (i) the samples have to be electrically charged, and (ii) we need electric and magnetic fields. Hence AMS does not work for neutral particles (atoms, molecules). In contrast, since IMS uses quantum interference for sorting, it works also for neutral samples. More importantly, since IMS does not use electromagnetic fields, it dispenses with bulky magnets.

**Measurement.** AMS measures only the mass-to-charge ratio  $m/q$  since it uses the Lorentz force. In contrast, IMS measures directly the mass  $m$ .

**Velocity regime.** In AMS the separation between mass species is proportional to the velocity. Thus, in order to achieve a good separation between mass species, AMS uses accelerators (e.g., TANDEM). In contrast, IMS works in the low-velocity regime, so accelerators are not necessary. Consequently, IMS can lead to compact devices, with low size and weight. This opens the possibility of portable mass spectrometers for field work.

**Velocity filters.** Both methods use velocity filters. Since IMS works in the low-velocity regime, one can use mechanical choppers. In contrast, mechanical choppers cannot be used

in the high-velocity regime of AMS, as they would introduce large errors.

	AMS	IMS
quantum behaviour	particle	wave
trajectory	localised	delocalised
separation mechanism	Lorentz force	interference
measurement	$m/q$	$m$
separation	$\sim v$	$\sim v^{-1}$
velocity regime	large $v$	small $v$

TABLE I: Complementarity between accelerator mass spectrometry (AMS) and interferometric mass spectrometry (IMS).

In conclusion, due to this complementarity IMS can potentially be used for applications where AMS is impractical. These include sensitive samples (e.g., biological, proteins) that break upon acceleration (or at the stripping phase in TANDEM) and neutral samples which are difficult to ionise. Moreover, since accelerators are not required, we envisage that IMS will lead to compact devices for mobile applications.

*Acknowledgments.* I'm grateful to Rareş Şuvăilă for many stimulating discussions. This work has been supported from a grant of the Romanian Ministry of Research and Innovation, PCCDI-UEFISCDI, Project Number PN-III-P1-1.2-PCCDI-2017-0338/79PCCDI/2018, within PNCDI III, and from PN 19060101/2019-2022.

- [1] R.A. Muller, *Radioisotope Dating with a Cyclotron*, Science **196**, 489 (1977).
- [2] L. Marton, *Electron Interferometer*, Phys. Rev. **85**, 1057 (1952).
- [3] L. Marton, J. Arol Simpson, J.A. Suddeth, *An Electron Interferometer*, Rev. Sci. Instruments **25**, 1099 (1954).
- [4] D.A. Pushin, M.G. Huber, M. Arif, D.G. Cory, *Experimental realization of decoherence-free subspace in neutron interferometry*, Phys. Rev. Lett. **107**, 150401 (2011).
- [5] E.M. Rasel, M.K. Oberthaler, H. Batelaan, J. Schmiedmayer, and A. Zeilinger, *Atom Wave Interferometry with Diffraction Gratings of Light*, Phys. Rev. Lett. **75**, 2633 (1995).
- [6] Klaus Hornberger, Stefan Gerlich, Philipp Haslinger, Stefan Nimmrichter, and Markus Arndt, *Colloquium: Quantum interference of clusters and molecules*, Rev. Mod. Phys. **84**, 157 (2012).
- [7] M. Arndt, O. Nairz, J. Vos-Andreae, C. Keller, G. van der Zouw, A. Zeilinger, *Wave-particle duality of C60 molecules*, Nature **401**, 680 (1999).
- [8] S. Gerlich, L. Hackermuller, K. Hornberger, A. Stibor, H. Ulbricht, M. Gring, F. Goldfarb, T. Savas, M. Muri, M. Mayor, M. Arndt, *A Kapitza-Dirac-Talbot-Lau interferometer for highly polarizable molecules*, Nature Physics **3**, 711 (2007).
- [9] C. Brand, F. Kialka, S. Troyer, C. Knobloch, K. Simonovic, B.A. Stickler, K. Hornberger, and M. Arndt, *Bragg diffraction of large organic molecules*, Phys. Rev. Lett. **125**, 033604 (2020).
- [10] Y.Y. Fein, P. Geyer, P. Zwick, F. Kialka, S. Pedalino, M. Mayor, S. Gerlich, M. Arndt, *Quantum superposition of molecules beyond 25 kDa*, Nature Physics **15**, 1242 (2019).
- [11] P. Geyer, U. Sezer, J. Rodewald, L. Mairhofer, N. Dorre, P. Haslinger, S. Eibenberger, C. Brand, M. Arndt, *Perspectives for quantum interference with biomolecules and biomolecular clusters*, Phys. Scr. **91**, 063007 (2016).
- [12] A. Shayeghi, P. Rieser, G. Richter, U. Sezer, J.H. Rodewald, P. Geyer, T. J. Martinez, M. Arndt, *Matter-wave interference of a native polypeptide*, Nature Communications **11**, 1447 (2020).
- [13] R. Ionicioiu, I. D'Amico, *Mesoscopic Stern-Gerlach device to polarize spin currents*, Phys. Rev. B **67**, 041307(R) (2003).
- [14] R. Ionicioiu, *Sorting quantum systems efficiently*, Sci. Rep. **6**, 25356 (2016).
- [15] X.B. Zou and W. Mathis, *Scheme for optical implementation of orbital angular momentum beam splitter of a light beam and its application in quantum information processing*, Phys. Rev. A **71**, 042324 (2005).
- [16] G.C.G. Berkhout, M.P.J. Lavery, J. Courtial, M.W. Beijersbergen, M.J. Padgett, *Efficient sorting of orbital angular momentum states of light*, Phys. Rev. Lett. **105**, 153601 (2010).
- [17] M. Mirhosseini, M. Malik, Z. Shi, R.W. Boyd, *Efficient separation of the orbital angular momentum eigenstates of light*, Nat. Commun. **4**:2781, doi:10.1038/ncomms3781 (2013).
- [18] Y. Zhou, M. Mirhosseini, D. Fu, J. Zhao, S.M. Hashemi Rafsanjani, A.E. Willner, and R.W. Boyd, *Sorting Photons by Radial Quantum Number*, Phys. Rev. Lett. **119**, 263602 (2017).
- [19] X. Gu, M. Krenn, M. Erhard, and A. Zeilinger, *Gouy Phase Radial Mode Sorter for Light: Concepts and Experiments*, Phys. Rev. Lett. **120**, 103601 (2018).
- [20] <https://www.physikinstrumente.com/en/products/nanopositioning-piezo-flexure-stages/multi-axis-piezo-flexure-stages/>
- [21] V.J. Lopez-Pastor, J.S. Lundeen, F. Marquardt, *Arbitrary optical wave evolution with Fourier transforms and phase masks*, arXiv:1912.04721.
- [22] M. Bachmann, P.A. Besse, H. Melchior, *General self-imaging properties in  $N \times N$  multimode interference couplers including phase relations*, Appl. Opt. **33**, 3905 (1994).
- [23] J. Zhou, *All-Optical Discrete Fourier Transform Based on Multimode Interference Couplers*, IEEE Photonics Technology Letters **22**, 1093 (2010).